



5. CABLE IDENTIFICATION: IDENTIFY PER STATEMENT OF WORK.
6. ALL HELI-COIL HOLES TO BE PREPARED ACCORDING TO EMHART HELI-COIL PRODUCT CATALOG, HC2000, REV 4
7. ALL HELI-COIL INSERTS TO BE INSTALLED BY LIGO PERSONNEL. AFTER DELIVERY OF FINISHED PARTS, USE NITRONIC 60 THREADED INSERTS.
8. MATERIAL:
- a. J1 CONNECTOR SHELL - GOLD OVER ELECTRO-LESS NICKEL SELECTIVELY METALIZED PEEK VICTREX 450GL30.
  - b. J2 CONNECTOR SHELL - GLENAIR PART NO. 600-052
  - c. BACKSHELL - STAINLESS STEEL WITH VENT HOLE.
  - d. CONTACTS - BERYLLIUM COPPER ALLOY C17300, 0.000050 MIN. GOLD OVER NICKEL.
  - e. HARDWARE: STAINLESS STEEL, PASSIVATED.
  - f. PEEK BRAID - PEEK VICTREX GRADE TDS-450CA30 CARBON LOADED.
9. CABLE: 6 COND. 22 AWG, (150/44), WITH .005 PFA INSULATION (COONER WIRE #CZ2205) 3 TWISTED PAIRS ( APPROX. 2 TWISTS PER INCH ) OVERALL 40AWG COPPER BRAID 50% COVERAGE. OVERALL PEEK BRAID MIN. 50% COVERAGE. OVERALL CABLE O.D. WILL BE APPROX. 0.240 IN.
10. CONNECTORS WILL BE SUPPLIED WITH HARDWARE. LENGTH OF SCREWS SHOULD BE THE PROPER LENGTH FOR MATING.
11. INDICATED LENGTH IS FROM CONNECTOR END TO CONNECTOR END. USE APPROPRIATE LENGTH TO COMPENSATE FOR THE INTERNAL WIRING OF THE CONNECTORS AND STRIP LENGTH.
12. INDICATED DIMENSIONS SHOWN FOR REFERENCE ONLY.
13. FILL UNUSED CONTACT POSITIONS WITH UNCRIMPED CONTACTS.
14. PART NO. SHOWN CORRESPONDS TO UNPLATED PARTS. MATERIALS/FINISH AS SPECIFIED ON NOTE 8, SHALL TAKE PRECEDENCE AT ALL TIMES.

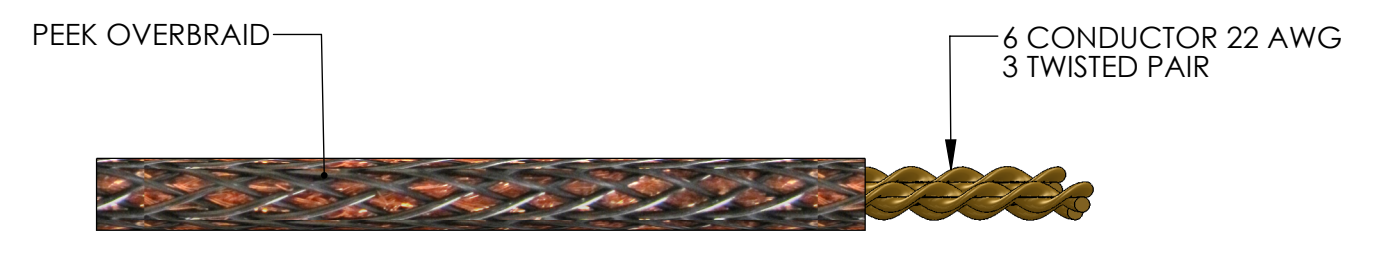


CABLE DETAIL

ISC TRANSMON BEAM DIVERTER CABLE SUSPENDED TRANSMON TABLE TO BEAM DIVERTER		
V25AB-36 - V-DB25HD M/S1-36-MM7PINHD F/X		
STANDARD USE FOR THIS CABLE		
SUBSYSTEM	AIR/VAC	STANDARD USE
ISC	IN-VAC	TRANSMON BEAM DIVERTER

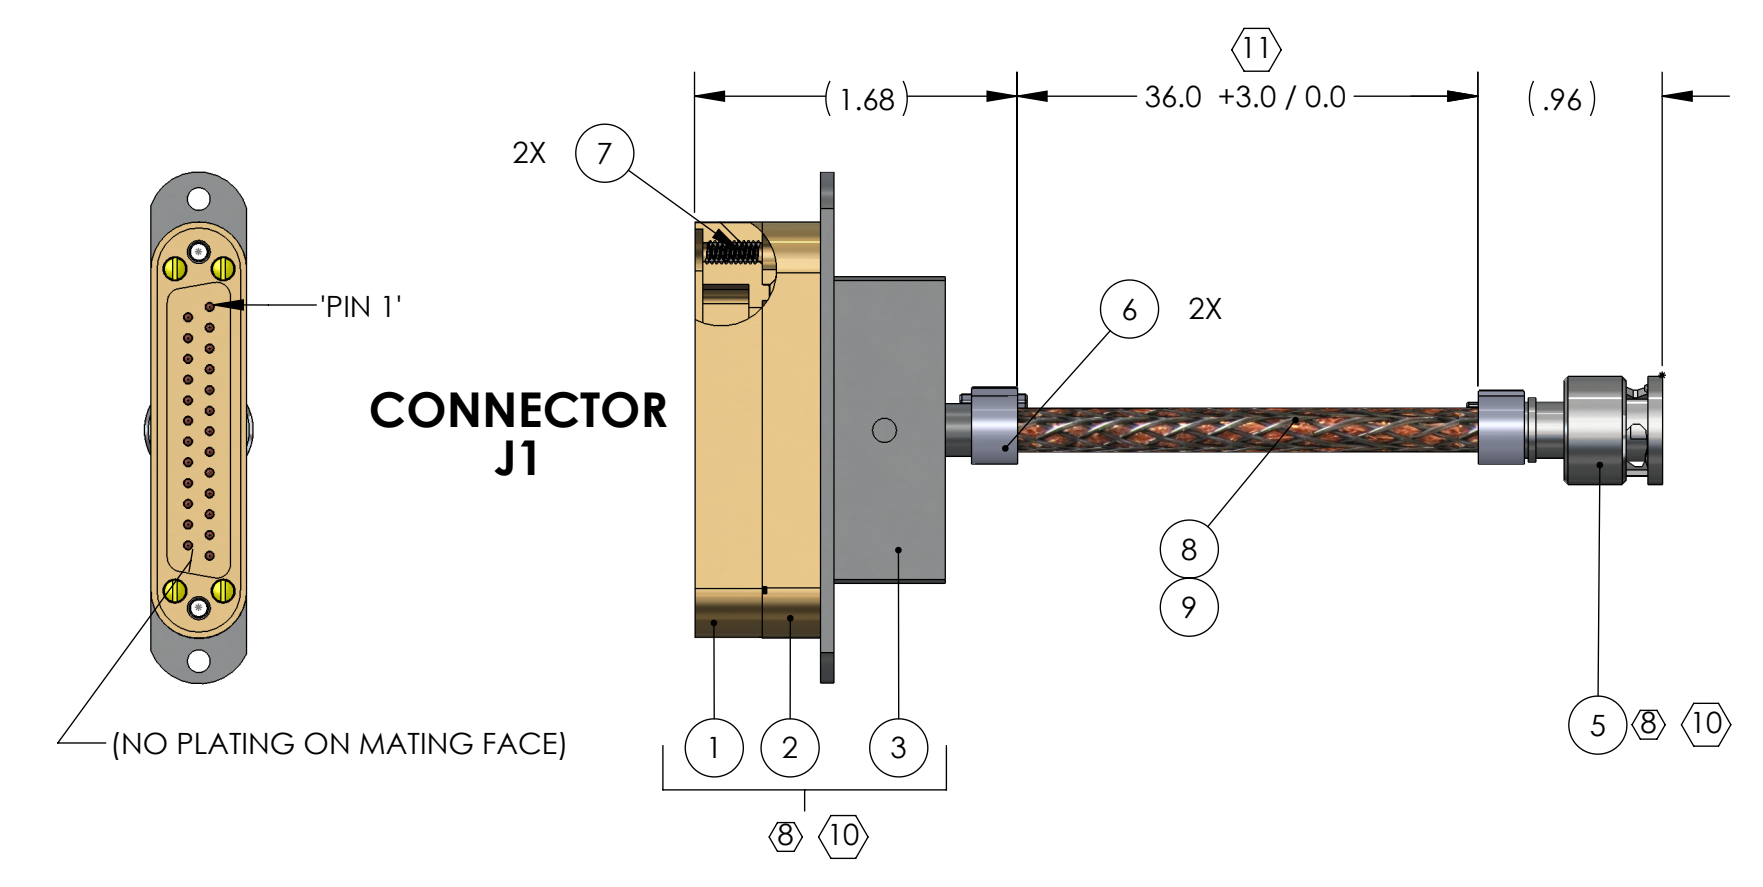




CONNECTOR J2

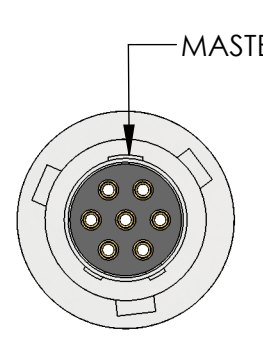


ROTATED 90 DEGREES CW  
(MATES WITH GLENAIR 803-003-07M6-7PN-598A)

REV.	DATE	DCN #	DRAWING TREE #
v1	11 FEB 2011	-	-
v7	16 JUL 2012	E1200711-v1	-
v8	14 AUG 2012	E1200757-x0	-

CONNECTOR 'J1' 8 10 12 13

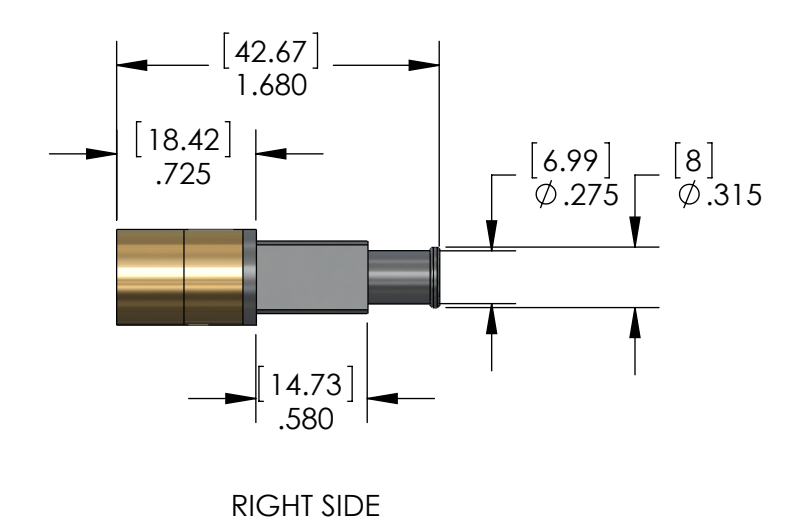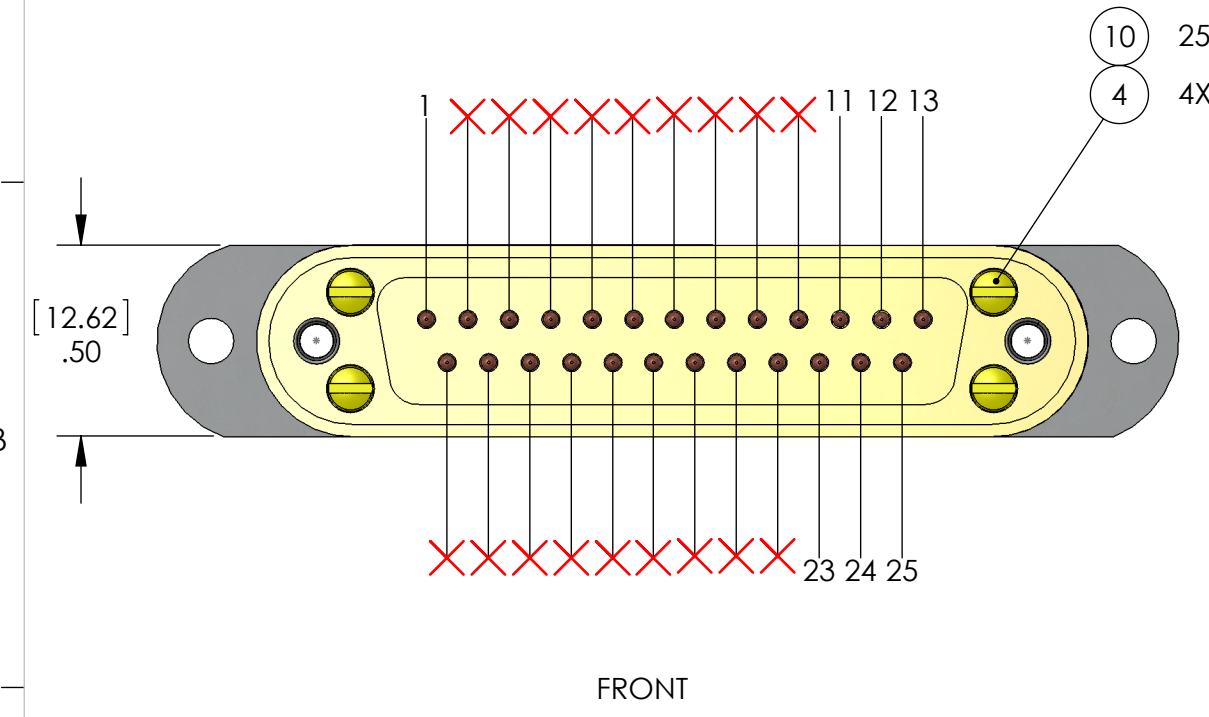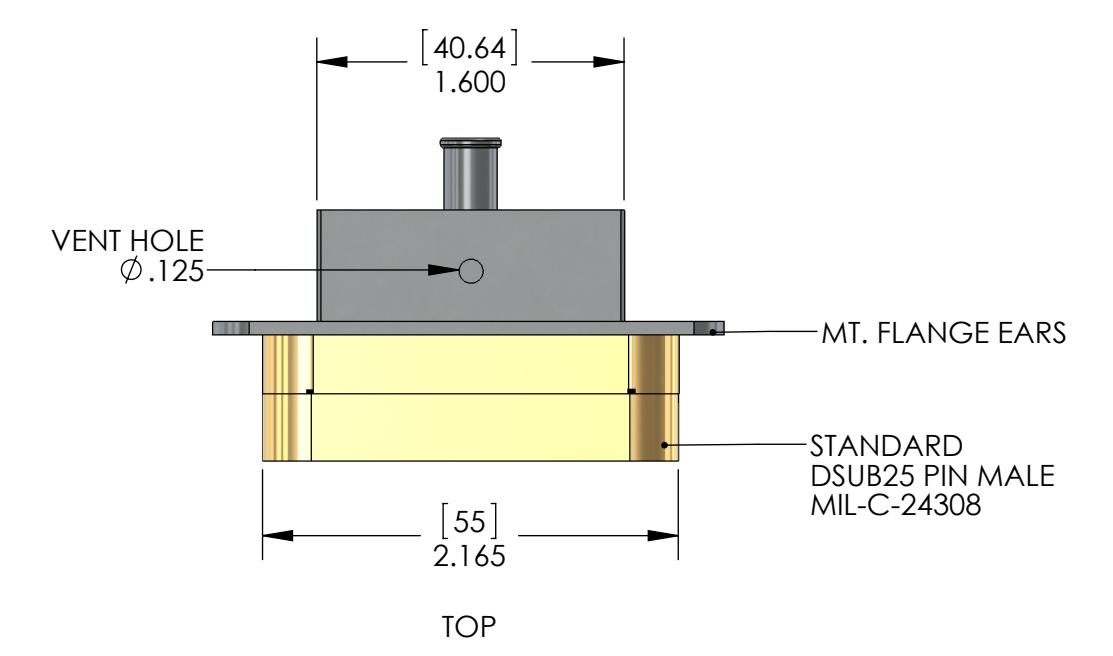

CONNECTOR 'J2' 8 10 13

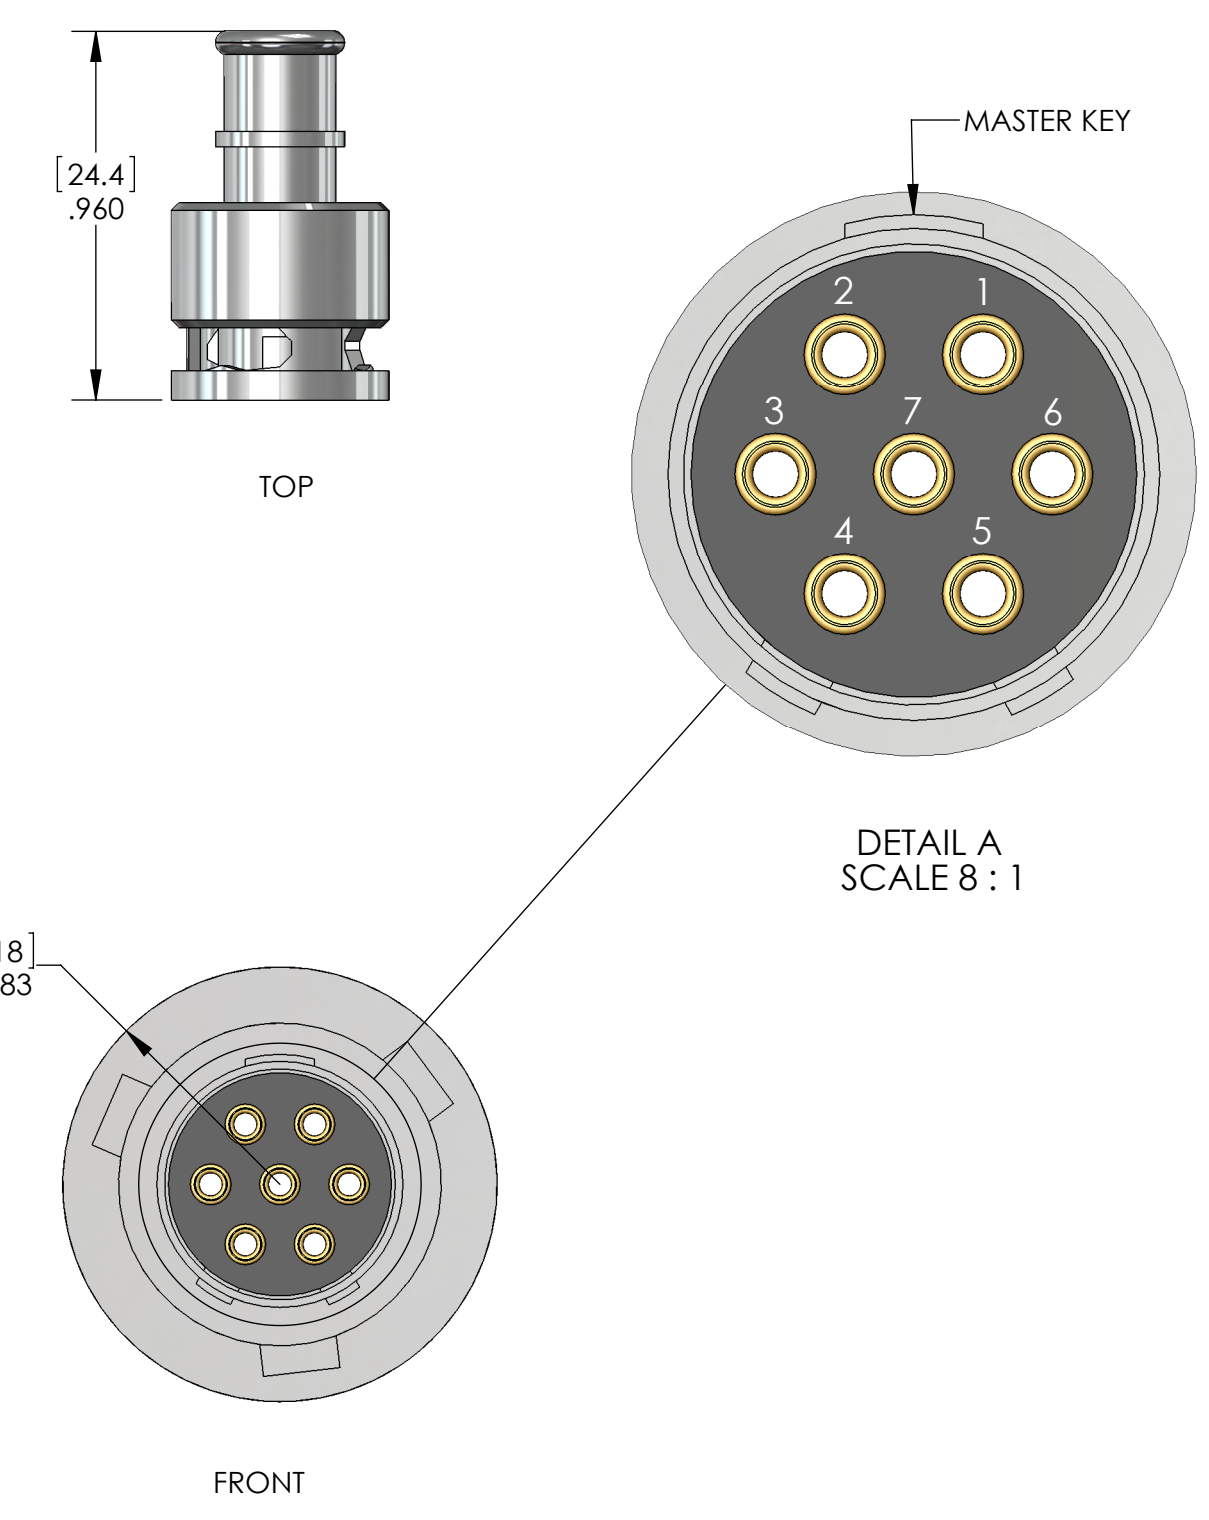

V25AB-36 CABLE ASSEMBLY CIRCUIT SUMMARY

FROM 'J1'		TO 'J2'		
PIN	WIRE NAME	TWISTED PAIR	PIN	SIGNAL
1	(SHIELD)		N/C	-
13	WIRE 13	TP-1	1	(+)COIL
25	WIRE 25		2	(-)COIL
12	WIRE 12	TP-2	3	(+)LEFT SENSOR
24	WIRE 24		4	(-)LEFT SENSOR
11	WIRE 11	TP-3	5	(+)RIGHT SENSOR
23	WIRE 23		6	(-)RIGHT SENSOR
N/C	-	-	7	N/C

TEST LIST	
FROM 'J1'	TO 'J2'
PIN	PIN
N/C	SHELL
SHELL	N/C
13	1
25	2
12	3
24	4
11	5
23	6
N/C	7

ITEM NO.	PART NUMBER	DESCRIPTION	MATERIAL	TOTAL
10	037-5001-2022 TICOR OR EQ.	SIZE 20 PIN CONTACT, 22D CRIMP BARREL	SEE NOTE 8	25
9	6759	PEEK OVERBRAID, 50% COVERAGE MIN.	ZEUS, .016 BLK PEEK DRAWN MONOFILAMENT	A/R
8	CZ2205 COONER WIRE	WIRE, 22 AWG (150/54)	SEE NOTE 9	A/R
7	1185-04EN-336	HELICOIL, 4-40 X .336 LG., NITRONIC60	NITRONIC 60	2
6	600-052 GLENAIR OR EQ.	BRAID CLAMPING BAND, .24 WIDE	ST. STEEL, PASSIVATED	2
5	803-001-06M6-7SN-598A GLENAIR	CONNECTOR, 7 PIN MIGHTY MOUSE SOCKET		1
4	013-2701-0001 TICOR OR EQ.	SCREW, FILLISTER HEAD, 1-72 X .450 LG., SLOTTED	SEE NOTE 8	4
3		UHV DSUB25 CONNECTOR BACKSHELL, W/ EARS		1
2	034-1002-2520 TICOR OR EQ.	CONTACT RETAINER, DSUB25, UHV, SHIELDED		1
1	034-1006-2520 TICOR OR EQ.	CONNECTOR INTERFACE, DSUB25, UHV, SHIELDED (MALE)		1
		PARTS LIST		

NOTES AND TOLERANCES: (UNLESS OTHERWISE SPECIFIED)	
1. INTERPRET DRAWING PER ASME Y14.5-1994.	
2. REMOVE ALL SHARP EDGES, .005-.015, FOR MACHINED PARTS. ROUND ALL EDGES APPROXIMATELY R.02 FOR SHEET METAL PARTS.	
3. DO NOT SCALE FROM DRAWING.	
4. ALL MACHINING FLUIDS MUST BE FULLY SYNTHETIC, FULLY WATER SOLUBLE AND FREE OF SULFUR, SILICONE, AND CHLORINE.	
DIMENSIONS ARE IN INCHES	
TOLERANCES:	
.XX ± .10	
.XXX ± .005	
ANGULAR ± .5°	
MATERIAL	N/A
FINISH	N/A μinch

CALIFORNIA INSTITUTE OF TECHNOLOGY MASSACHUSETTS INSTITUTE OF TECHNOLOGY		PART NAME	
SYSTEM		CUSTOM CABLE SPECIFICATION, V25AB-36	
ADVANCED LIGO	SUB-SYSTEM	DESIGNER	B.ABBOT 11 FEB 2011
	ISC	DRAFTER	E.BROWN 11 FEB 2011
NEXT ASSY	N/A	CHECKER	SEE DCC
		APPROVAL	SEE DCC
		SIZE	D
		DWG. NO.	D1000237
		REVISION	v8
		SCALE:	NTS
		PROJECTION:	1st Angle
		SHEET 1 OF 1	

D1000237 LIGO, ITC, CUSTOM CABLE SPECIFICATION V25AB-36, PART PDM REV: X-001, DRAWING PDM REV: X-009