



Analysis of LIGO Test Mass Internal Modes as a Measure of Coating Absorption

Greg McIvor
Sam Waldman
Phil Willems


September 21st, 2007
LIGO DetChar Telecon

LIGO-G070636-00-0


Test Mass Body Modes

- 25 cm diameter, 10 cm thick, 10 kg, fused silica
 - » Calculate modes using finite element analysis
- Frequency of modes changes with temperature
 - » Temp dependence of Young's modulus
 - » $df / f = 70 \text{ ppm} / \text{K}$
- Frequency shift of the test mass body modes gives a measure of the temperature of the mirrors
 - » Temperature change due to absorption driven by IFO / TCS power step
 - » Coating absorption seems to be larger (by factor of $\sim 5-10$) than when initially measured in the lab at CalTech
 - » Track motion of modes vs. time throughout S5 data

“Drumhead” Mode

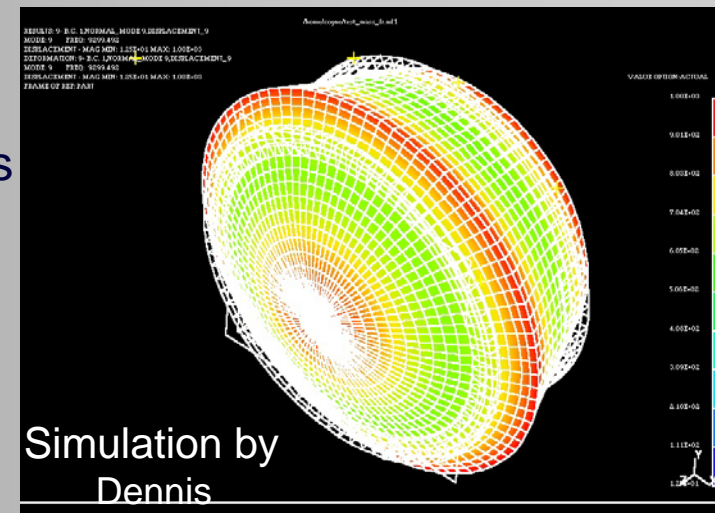





Visible in LIGO data

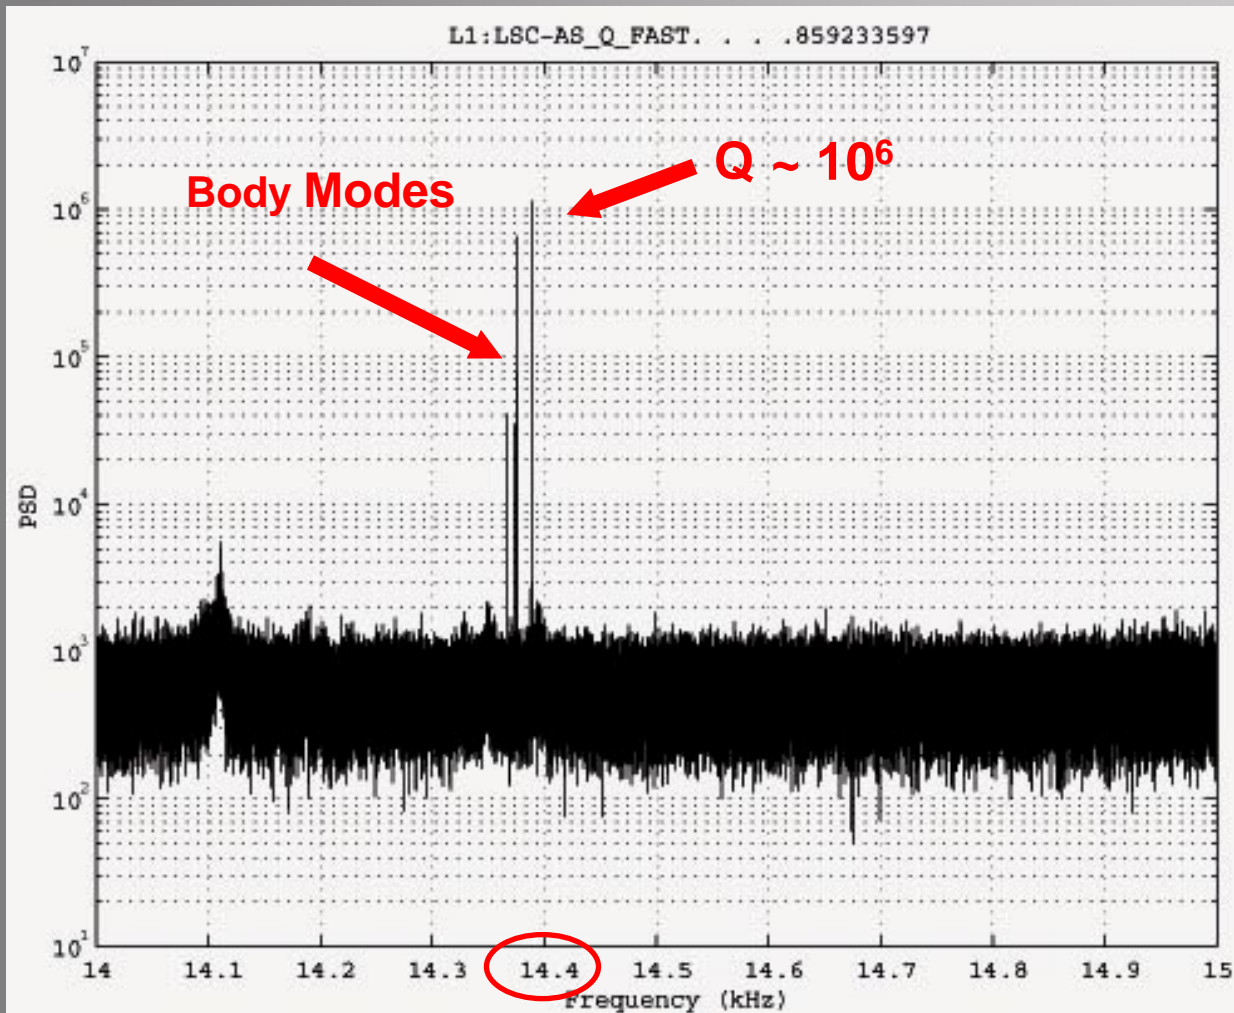


Computational Issues

- ~2 Years of Data, stored on tape
 - » Slow to access
- Want to extract only the 256kHz “FAST” Channel
 - » Store data on disk to perform analysis
- 256kHz sample rate yields huge amount of data
 - » Need to reduce amount of data stored
- Solution: heterodyne and downsample time series
 - » Generate “reduced” frame files

Heterodyne Windows

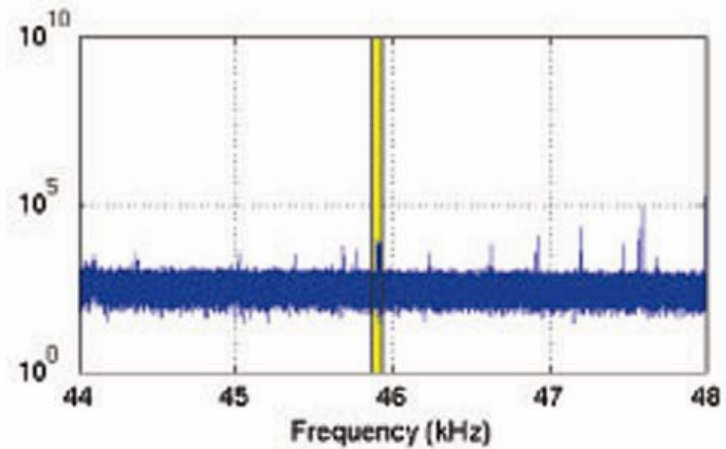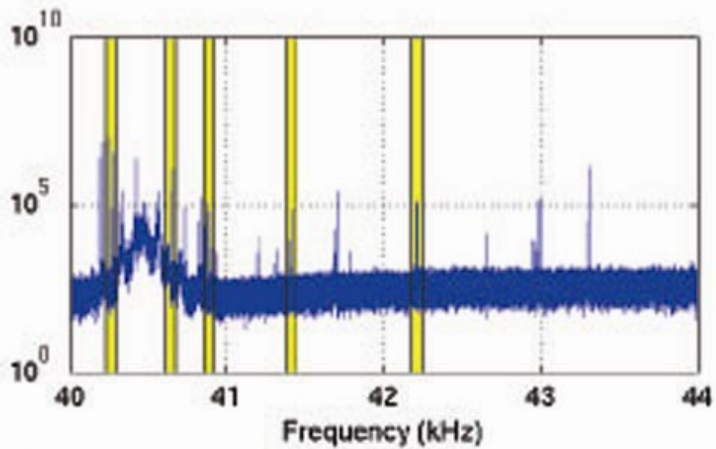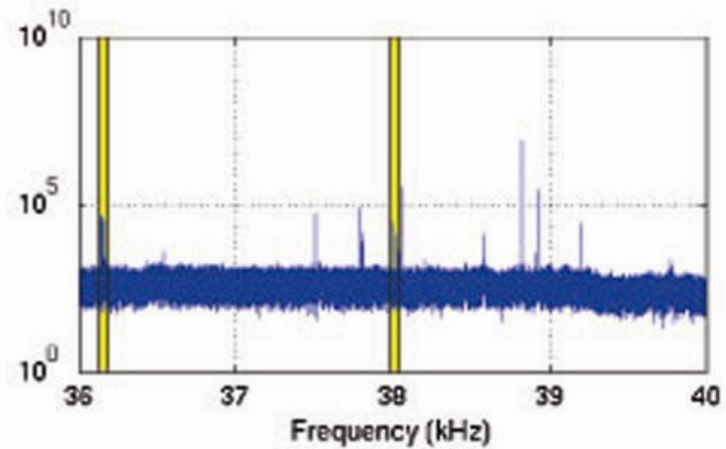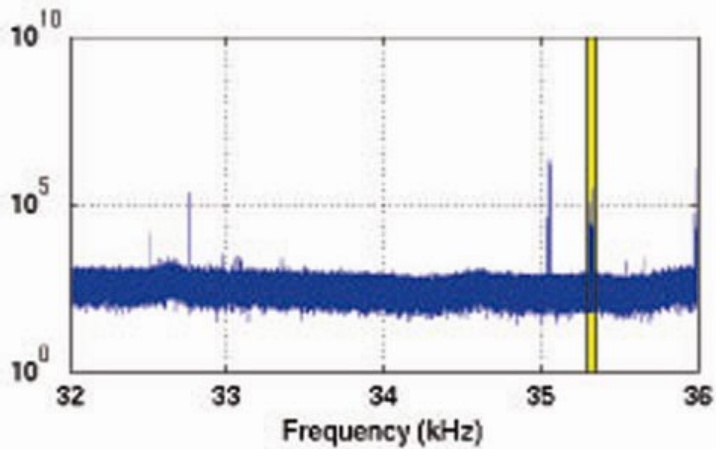

Full / Heterodyned Comparison

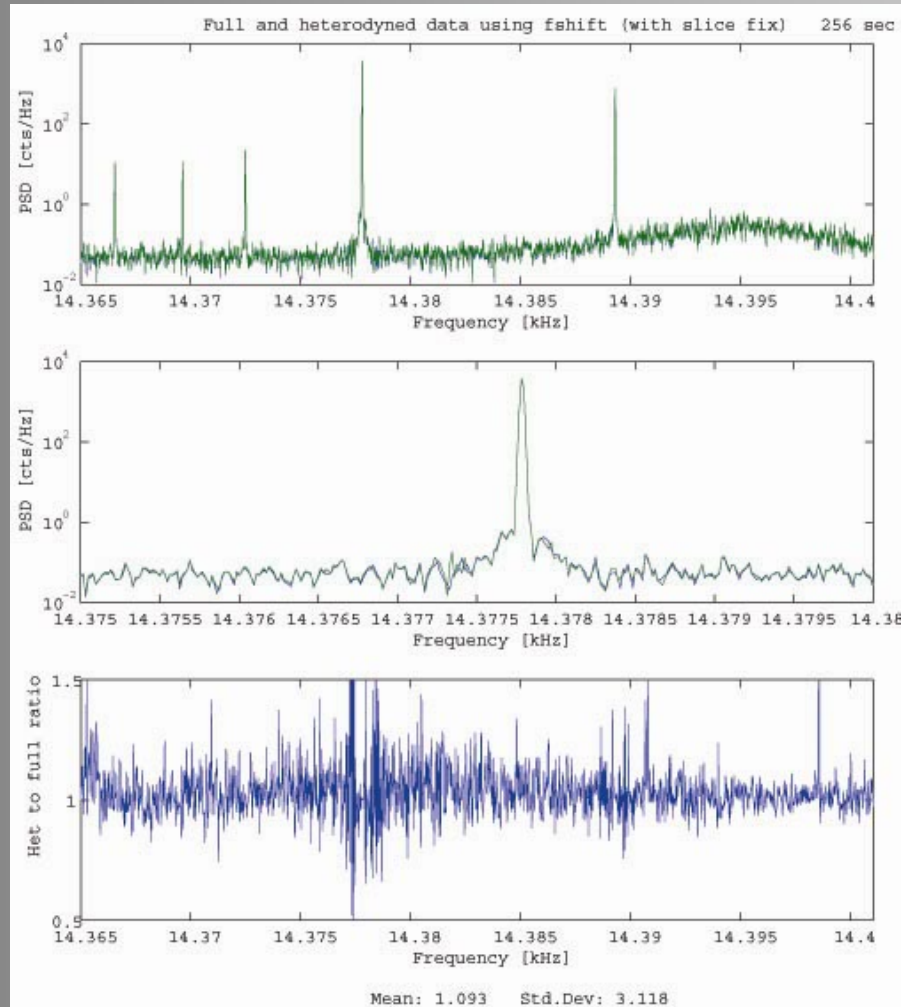

Computational Procedure

- FFT heterodyned time series stored in new frames
 - » Repeat for each channel
- Fit peaks with Lorentzian
 - » Accurately determine center frequency

$$L(x) = \frac{A}{2\pi} \frac{\Gamma}{(x - x_0)^2 + (\frac{1}{2}\Gamma)^2} + y_0$$


- Γ - Full Width Half Max
- x_0 - Center Frequency
- A - Overall Scale Factor
- y_0 - Vertical Shift

Toolboxes used / Bugs Found

- Use GDS libraries for frame generation
 - » Libframe – frame access / generation
 - Found N+1 Bug
 - » fShift – heterodyne time series
 - Long time series accumulate error from FIR filter
 - » DecimateBy2 – downsample heterodyned time series

- Use Matlab for peak finding / analysis
 - » Pwelch() – 8 averaged overlapping FFT with Hamming window
 - » Fmincon() – fit Lorentzian using least squares minimization


Simulation

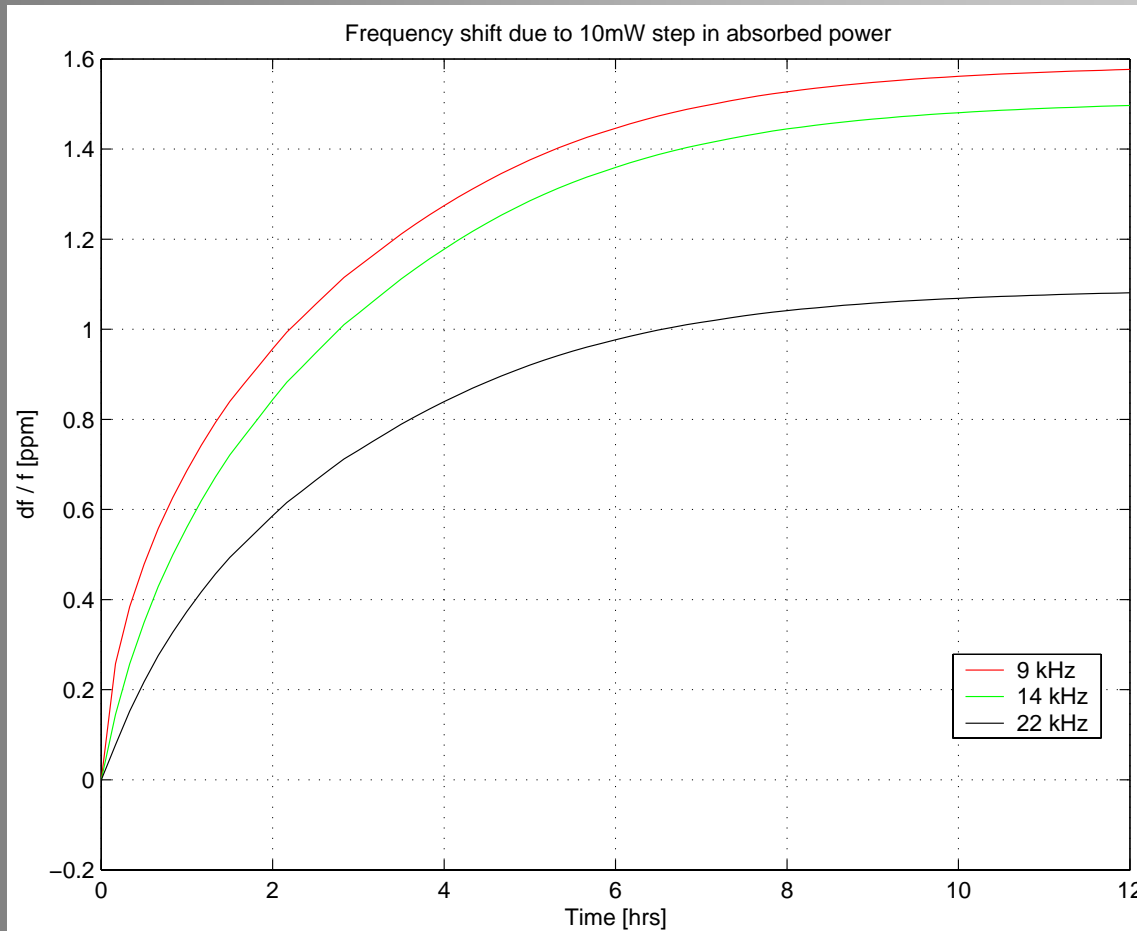

Comsol finite element analysis simulation by Phil Willems

Results


Calculated absorption:
 < 5ppm
 Up to 30% error

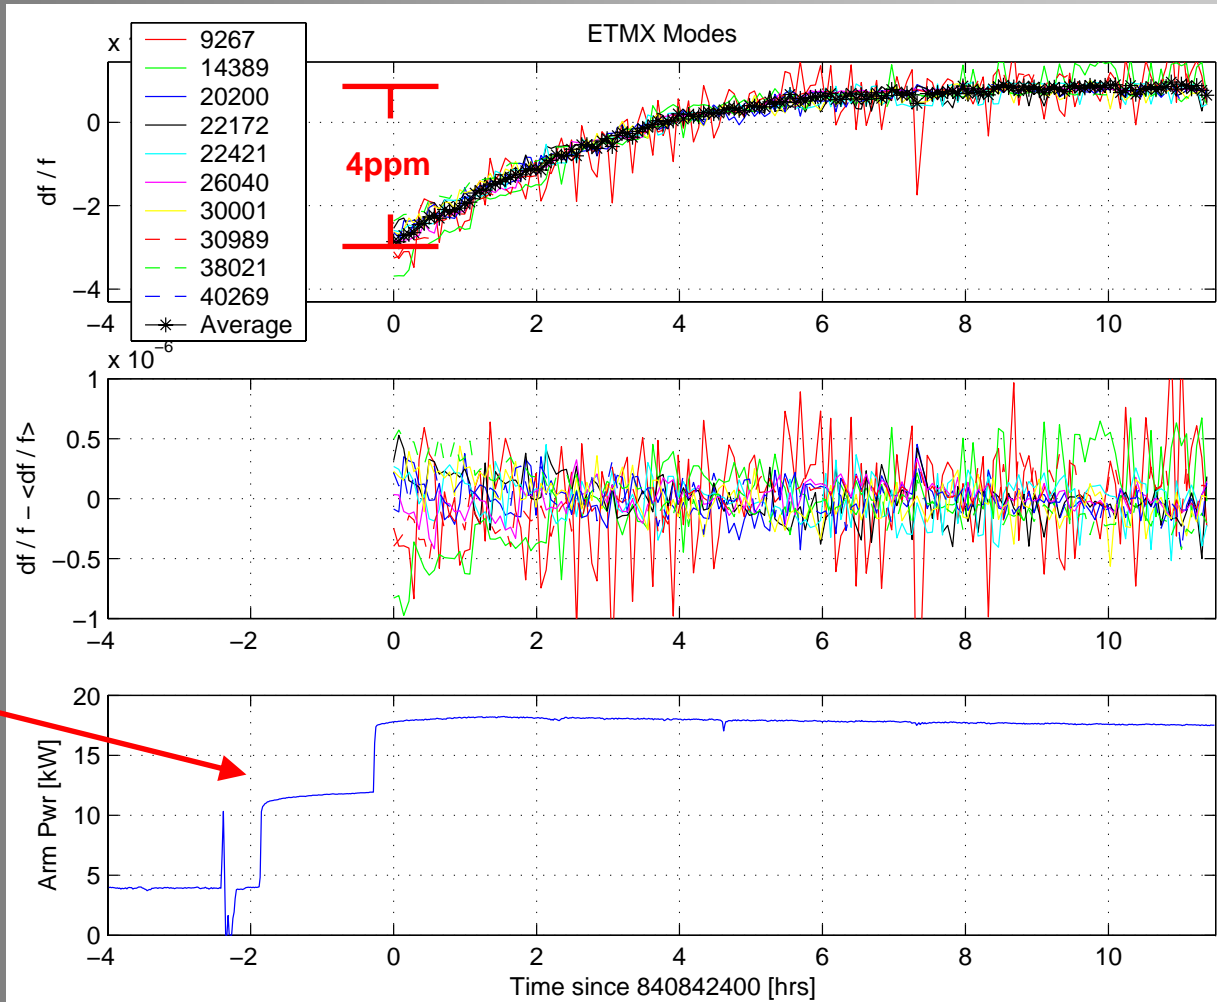

Complicated initial conditions

Ambient Temperature Drift


30 mK
Temperature
Shift

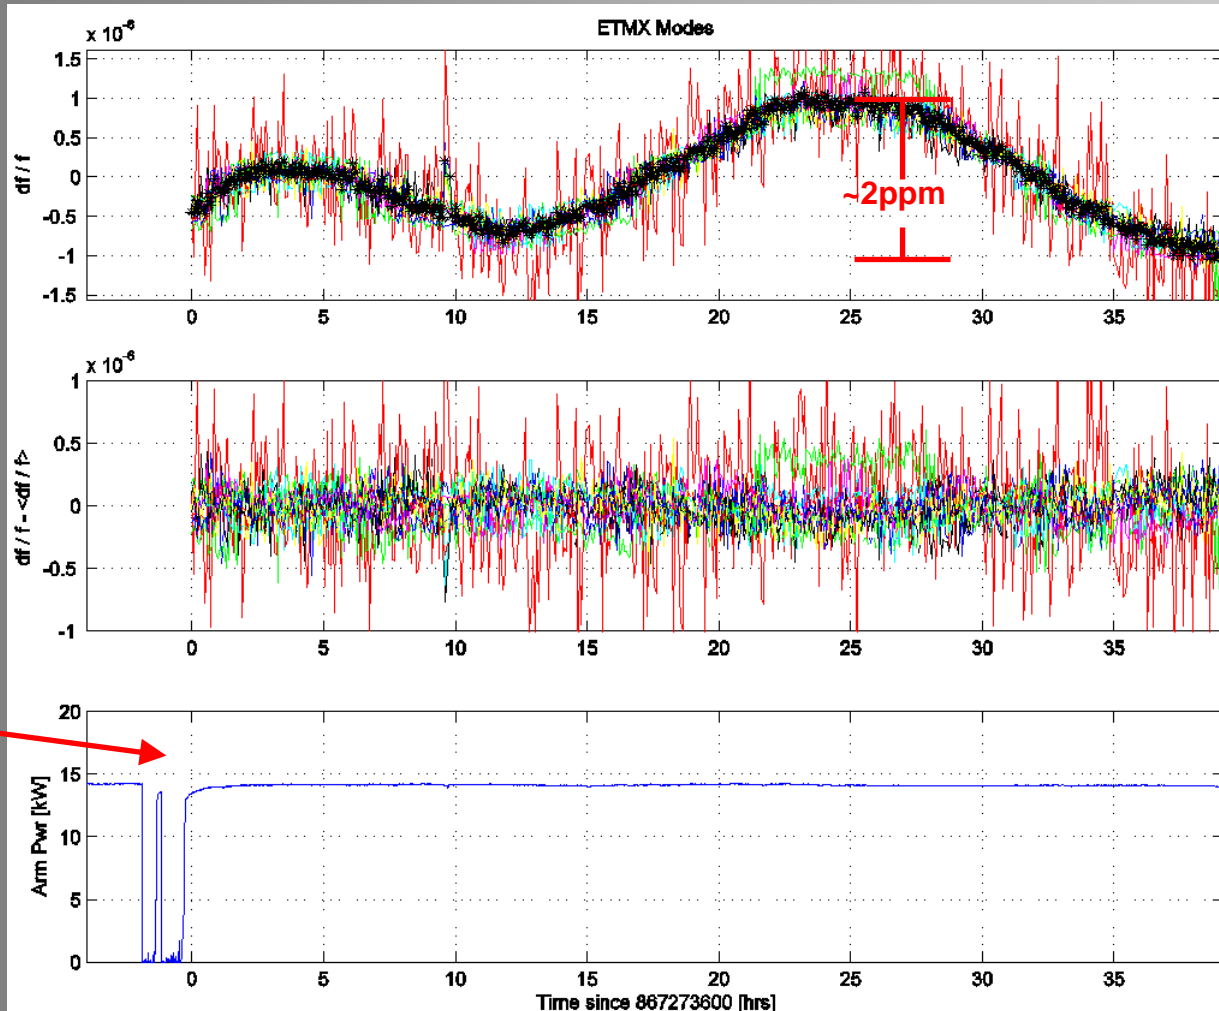

Steady State

Absorption / Ambient


Calculated absorption:
 < 3.5 ppm
 Up to 10% error

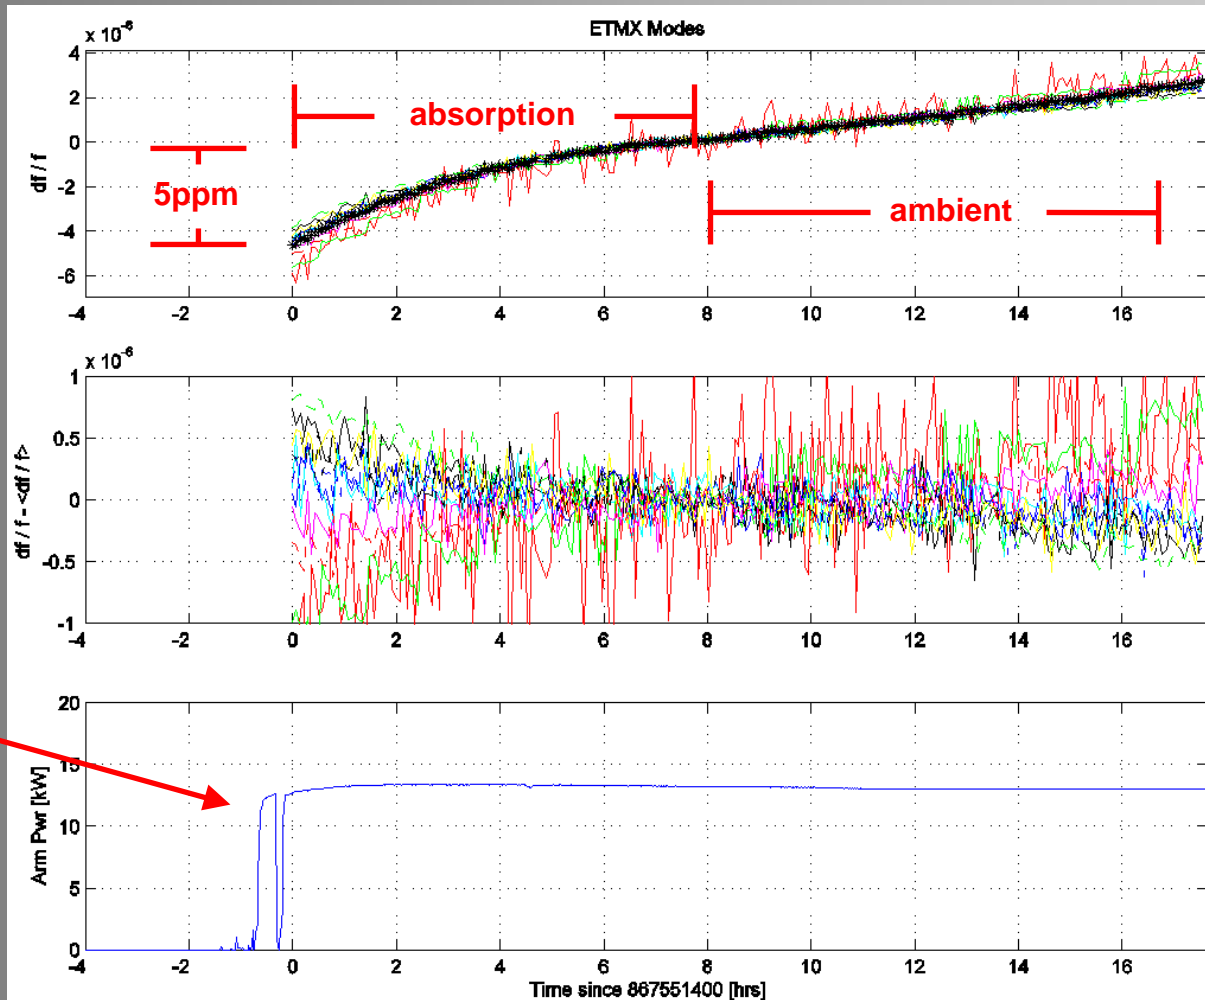

Good power step

Temperature Data

Calculated absorption:
 < 3.5 ppm
 Up to 30% error

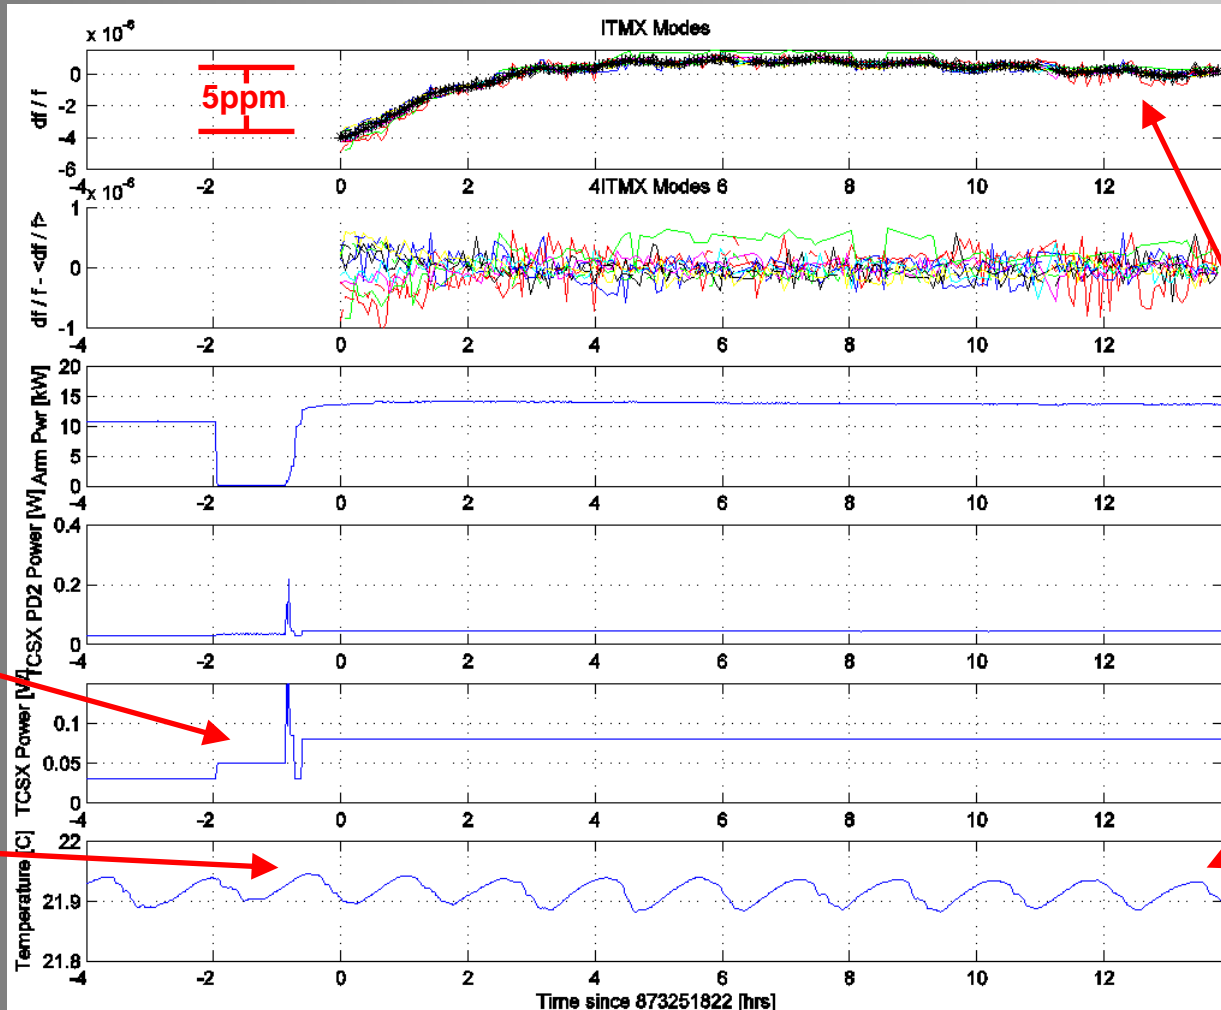


TCS step

Steady avg. Temp

~1.5 hr Temp fluctutaions

Temperature Data

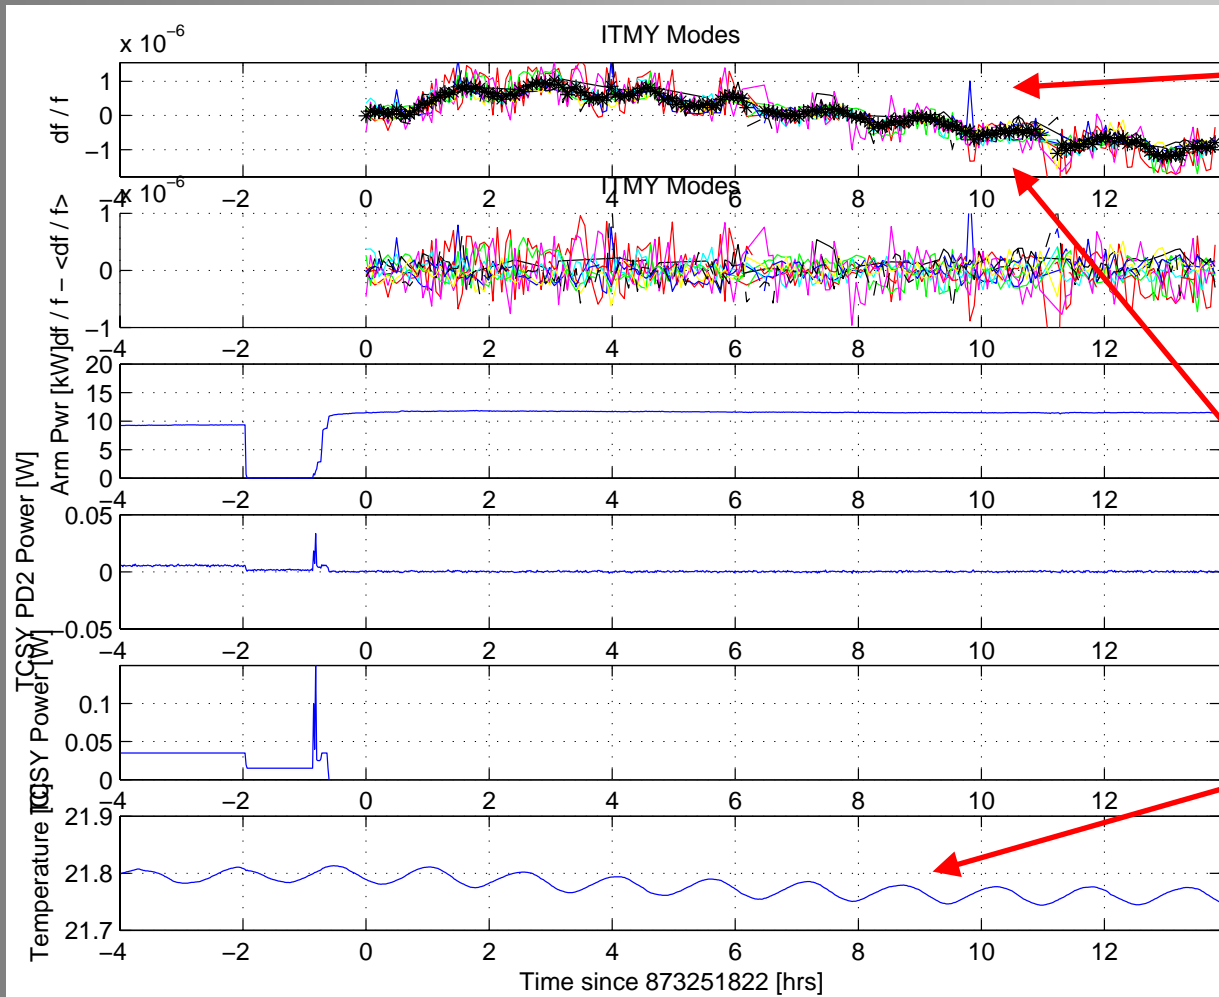

Temp induced shift:
~ 1.5 ppm

Decreasing avg. Temp
~ 20 mK

Post S5 Commissioning

- New temperature sensors installed at LLO by Phil allow for removal of ambient temperature induced frequency shift
 - » ITM sensors recently connected
 - » ETM temperature sensors still need to be connected!
- Need >5 hour lock segments for good absorption measurement
 - » 1W Mode cleaner power step
- Vary TCS power for verification
 - » Use Annulus / Central Heating for mode spectroscopy
- Perform analysis on H2 while upgrade in progress
 - » Before / after each vent

Summary

- Analysis of internal mode frequency shift can yield very accurate measure of absorption
 - » limited by systematic error
- Need long lock segment with power step
 - » Post S5 commissioning perfect opportunity
- Ambient temperature induced shifts can be removed for ITM
 - » Need ETM temperature sensors
- Absolutely necessary to understand for AdLIGO
 - » Power in arms 50x larger than initial LIGO
- Changing absorption would be serious problem