
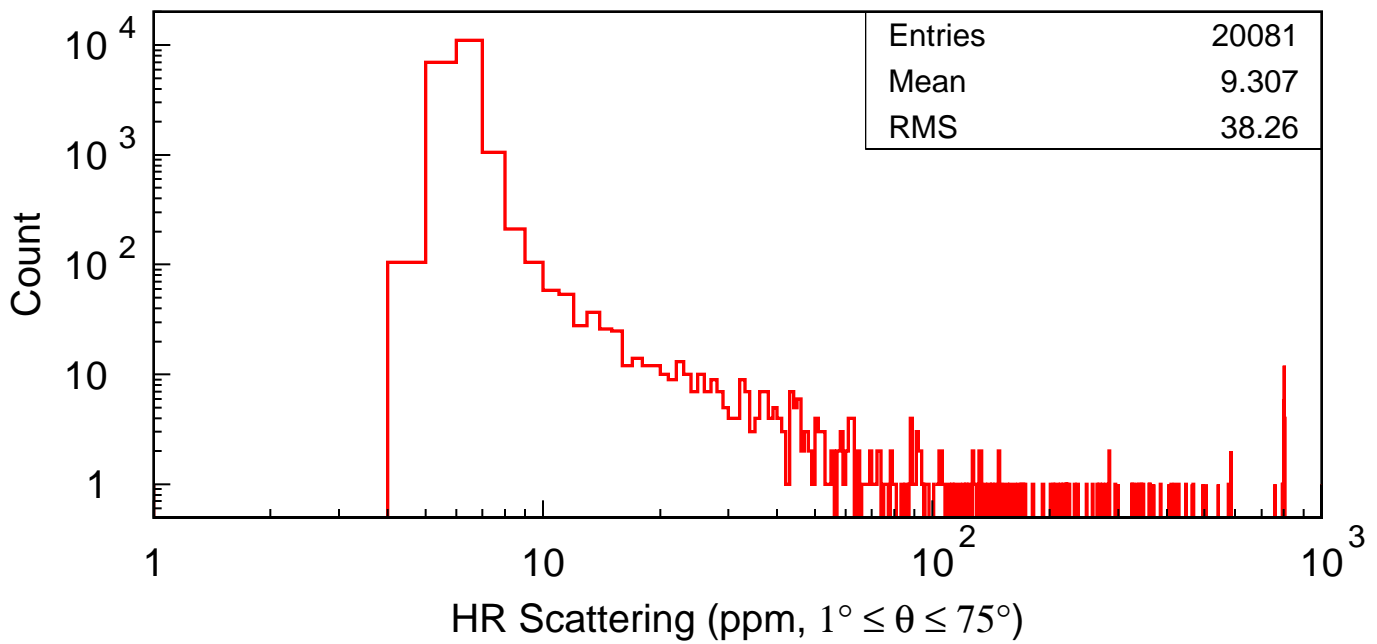


ETM12 HR TIS measurement, 072122

($\phi_{\text{beam}} = 0.3 \text{ mm}$, Step= 1.0 mm)

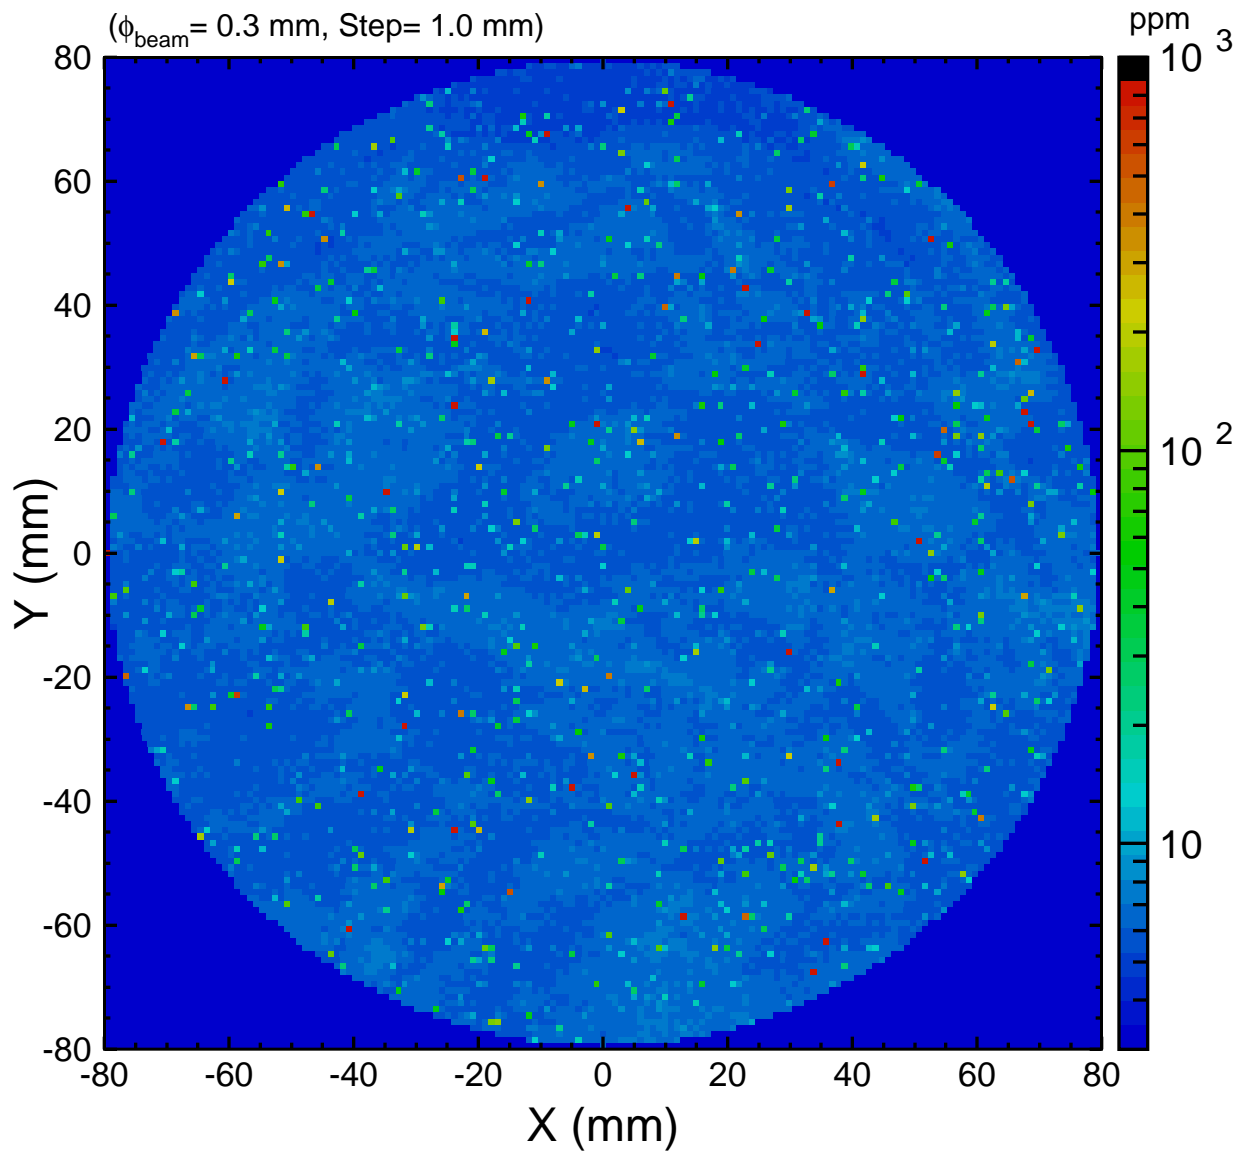

ETM12 HR TIS measurement, 072322

($\phi_{\text{beam}} = 0.3 \text{ mm}$, Step= 0.3 mm)

