

# Validating gravitational-wave detections: The Advanced LIGO hardware injection system

C. Biwer,<sup>1</sup> J. Betzwieser,<sup>2</sup> R. P. Fisher,<sup>1</sup> E. Goetz,<sup>3</sup> S. Kandhasamy,<sup>2</sup> S. Karki,<sup>4</sup> J. S. Kissel,<sup>3</sup> A. P. Lundgren,<sup>5</sup> D. M. Macleod,<sup>2</sup> A. Mullavey,<sup>2</sup> K. Riles,<sup>6</sup> J. G. Rollins,<sup>7</sup> E. Thrane,<sup>8</sup> T. D. Abbott,<sup>9</sup> B. Allen,<sup>5,10,11</sup> D. A. Brown,<sup>1</sup> P. Charlton,<sup>12</sup> S. G. Crowder,<sup>13</sup> P. Fritschel,<sup>14</sup> J. B. Kanner,<sup>7</sup> C. Lazzaro,<sup>15,16</sup> M. Millhouse,<sup>17</sup> M. Pitkin,<sup>18</sup> R. L. Savage,<sup>3</sup> P. Shawhan,<sup>19</sup> D. H. Shoemaker,<sup>14</sup> J. R. Smith,<sup>20</sup> L. Sun,<sup>21</sup> J. Veitch,<sup>22</sup> S. Vitale,<sup>14</sup> A. J. Weinstein,<sup>7</sup> N. Cornish,<sup>17</sup> R. C. Essick,<sup>14</sup> M. Fays,<sup>23</sup> E. Katsavounidis,<sup>14</sup> J. Lange,<sup>24</sup> T. B. Littenberg,<sup>25</sup> R. Lynch,<sup>14</sup> P. M. Meyers,<sup>26</sup> F. Pannarale,<sup>23</sup> R. Prix,<sup>5</sup> R. O’Shaughnessy,<sup>24</sup> and D. Sigg<sup>3</sup>

<sup>1</sup>*Syracuse University, Syracuse, NY 13244, USA*

<sup>2</sup>*LIGO Livingston Observatory, Livingston, LA 70754, USA*

<sup>3</sup>*LIGO Hanford Observatory, Richland, WA 99354, USA*

<sup>4</sup>*University of Oregon, Eugene, OR 97403, USA*

<sup>5</sup>*Albert-Einstein-Institut, Max-Planck-Institut für Gravitationsphysik, D-30167 Hannover, Germany*

<sup>6</sup>*University of Michigan, Ann Arbor, MI 48109, USA*

<sup>7</sup>*LIGO, California Institute of Technology, Pasadena, CA 91125, USA*

<sup>8</sup>*Monash University, Victoria 3800, Australia*

<sup>9</sup>*Louisiana State University, Baton Rouge, LA 70803, USA*

<sup>10</sup>*University of Wisconsin-Milwaukee, Milwaukee, WI 53201, USA*

<sup>11</sup>*Leibniz Universität Hannover, D-30167 Hannover, Germany*

<sup>12</sup>*Charles Sturt University, Wagga Wagga, New South Wales 2678, Australia*

<sup>13</sup>*Bellevue College, Bellevue, WA 98008, USA*

<sup>14</sup>*LIGO, Massachusetts Institute of Technology, Cambridge, MA 02139, USA*

<sup>15</sup>*Center for Relativistic Astrophysics and School of Physics,  
Georgia Institute of Technology, Atlanta, GA 30332, USA*

<sup>16</sup>*INFN, Sezione di Padova, I-35131 Padova, Italy*

<sup>17</sup>*Montana State University, Bozeman, MT 59717, USA*

<sup>18</sup>*SUPA, University of Glasgow, Glasgow, G12 8QQ, United Kingdom*

<sup>19</sup>*University of Maryland, College Park, MD 20742, USA*

<sup>20</sup>*California State University Fullerton, Fullerton, CA 92831, USA*

<sup>21</sup>*The University of Melbourne, Parkville, Victoria 3010, Australia*

<sup>22</sup>*University of Birmingham, Birmingham, B15 2TT, United Kingdom*

<sup>23</sup>*Cardiff University, Cardiff CF24 3AA, United Kingdom*

<sup>24</sup>*Rochester Institute of Technology, Rochester, NY 14623, USA*

<sup>25</sup>*University of Alabama in Huntsville, Huntsville, AL 35899, USA*

<sup>26</sup>*University of Minnesota, Minneapolis, MN 55455, USA*

(Dated: October 25, 2016)

Hardware injections are simulated gravitational-wave signals added to the Laser Interferometer Gravitational-wave Observatory’s (LIGO) data. The detectors’ test masses are physically displaced by an actuator in order to simulate a gravitational wave. The simulated signal initiates a control-system response designed to mimic that of a true gravitational wave. Propagating a signal through the detector to the analyses provides an end-to-end test of LIGO’s ability to observe gravitational waves. The gravitational-wave analyses used to detect and characterize signals are tested with hardware injections. By looking for discrepancies between the recovered and injected signals, we are able to characterize the performance of analyses and the coupling of subsystems to the detectors’ output channel. Here we describe the LIGO hardware injection system and show the recovery of injected signals from binary black hole mergers, a stochastic gravitational-wave background, isolated pulsars, and detector characterization studies.

## I. INTRODUCTION

The Advanced Laser Interferometer Gravitational-Wave Observatory (aLIGO) is a network of two interferometric gravitational-wave detectors located in Hanford, WA, and Livingston, LA [1]. aLIGO is part of a global network of current and planned detectors including Virgo [2], GEO600 [3], KAGRA [4], and LIGO India [5]. The first direct observations of gravitational waves were made in aLIGO’s first observing run [6, 7].

These events were the first observations of binary black hole mergers [6, 7].

In order to make confident statements about gravitational-wave events, aLIGO employs studies to understand both transient and persistent noise artifacts [8], and the calibration of the detectors [9, 10]. In addition, detection and parameter estimation analyses have techniques to mitigate non-Gaussian noise in the detectors’ data [11, 12]. Part of testing these analyses and characterizing the detectors involves carrying out “hardware

injections” in which simulated gravitational-wave signals are added to the detector’s output channel. Hardware injections have several uses. Following a detection candidate, we study similar simulated gravitational-wave signals through the use of repeated injections. These hardware injections provide an end-to-end check for the search and parameter estimation analyses to recover signals in the detectors’ data. The recovery of hardware injections provide an additional check of the sign of the calibration between the aLIGO detectors using astrophysical waveforms and it is possible to measure the time delay of the signal in the controls system; the calibration of the detectors is checked by other means as well [9, 10]. In addition, we can check for cross-couplings in the controls system to the detectors’ output channel by identifying instrumental and environmental channels that are found to contain a trace of the injected signals.

Another use for hardware injection in Initial LIGO were “blind injections” which were hardware injections known only to a small team [13, 14]. Blind injections simulate the detection and characterization of a real astrophysical signal. No blind injections were carried out during aLIGO’s first observing run.

aLIGO measures the differential displacement along the two arms  $\Delta L = \delta L_x - \delta L_y$ , however, the output channel to analyses is gravitational-wave strain  $h = \Delta L/L$  where  $L = L_x = L_y$  [15]. The mirrors in the arms act as ‘freely falling’ test masses [15]. To add the hardware injection signal to the data we physically displace the detectors’ test masses in a way that mimics a gravitational-wave signal. In aLIGO’s first observing run, hardware injections were realized with two different actuation methods: electrostatic drive systems [16, 17] and photon radiation pressure actuators referred to as “photon calibrators” [18]. The photon calibrators are currently the only actuator used to perform hardware injections since their actuation range available for hardware injections is larger.

During aLIGO’s first observing run, astrophysical waveforms were injected using both actuation methods to test the detection and parameter estimation analyses. aLIGO is sensitive to a wide variety of astrophysical sources of gravitational waves including: binary black hole and/or neutron star mergers [19, 20], the stochastic gravitational-wave background [21], and isolated pulsars [22]. Hardware injections for each of these astrophysical sources were injected. In addition, series of sine-Gaussians were injected across the aLIGO frequency range to check for cross-couplings to the detectors’ output channel.

This paper describes how we inject signals into the aLIGO detectors with the photon calibrators in Section II. Section III describes the results from analyses that used hardware injections in aLIGO’s first observing run. This includes the recovery of binary black hole merger signals in Section III A and III B, the stochastic gravitational-wave hardware injection in Section III C, and a population of isolated pulsars in Section III D. A

description of the detector characterization analysis to check for cross-couplings to the detectors’ output channel is described in Section III E. Finally, Section IV summarizes the hardware injections and results from aLIGO’s first observing run.

## II. HARDWARE INJECTION PROCEDURE

Each astrophysical source has a different physical signal, and hence different technical requirements for the hardware injection system. In aLIGO’s frequency range, compact binary mergers can last a fraction of a second to minutes depending on the component masses. We begin our hardware injection waveforms at 15 Hz, and as the two component masses inspiral closer together they sweep upward in frequency [6]. The merger’s termination frequency is determined by the masses of the two objects. For example, GW150914 terminates at 250 Hz [6], however, the inspiral-only portion of a binary neutron star waveform with both component masses equal to  $1.4 M_\odot$  terminates at 1527 Hz. Isolated pulsars emit continuous gravitational waves at a particular frequency that is Doppler modulated by Earth’s motion and the gravitational-wave frequency slowly evolves as the pulsar spins down [22]. The stochastic background is the superposition of many events that combine to create a low-level signal [21]. Non-astrophysically motivated injections include a succession of short duration ( $< 1$  s) sine-Gaussians used to search for couplings with the detector output channel.

The difference in the time duration of the sources requires separate controls, so we categorize hardware injections into two classes: “transient injections” that are localized in time, and “continuous-wave injections” that are active throughout the duration of the observing run. Examples of transient injections include binary black hole and/or neutron star mergers, sine-Gaussians, and short-duration stochastic background signals; we increase the amplitude of the stochastic background waveform in order to limit it to a short segment of data. Continuous-wave injections are a population of isolated pulsars. Separate automation processes control transient and continuous-wave injections. Fig. 1 shows a schematic of the two pathways that generate and transmit gravitational-wave strain time series to the photon calibrator. In this section we work through Fig. 1, beginning at the top-left and working clockwise, in order to describe the processes that control the transient and continuous-wave injections.

We generate the simulated gravitational waveforms for transient injection signals prior to injection. The system for managing the automated processes of the aLIGO detector subsystems is Guardian [23]. Guardian manages the transient hardware injections and each automation step is recorded as a distinct state of the hardware injection subsystem. Guardian reads the next scheduled injection’s time series and transmits the data to the dig-

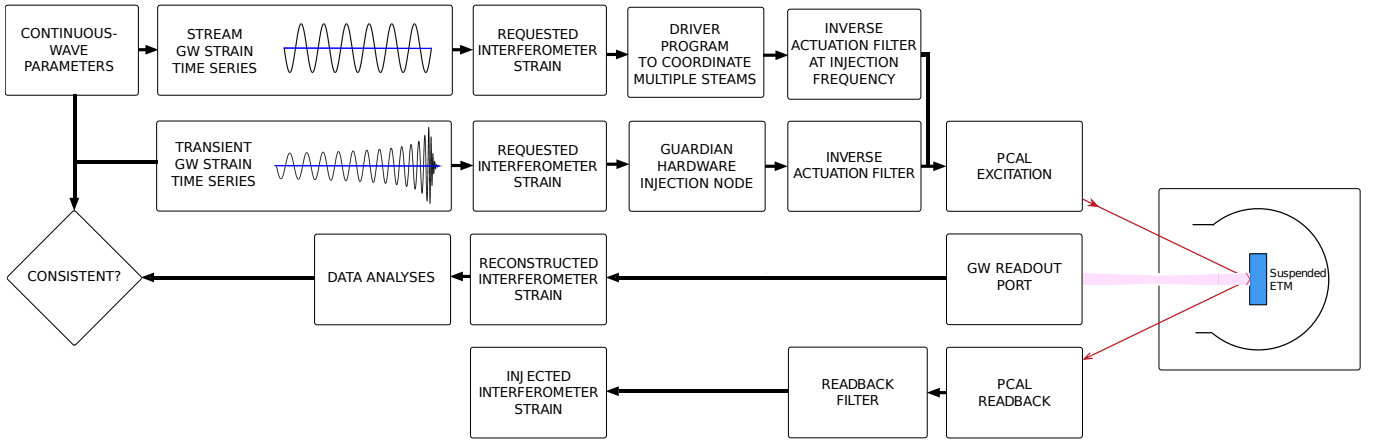


FIG. 1: Schematic diagram of the aLIGO hardware injection system. Time series for transient and continuous-wave injections are generated and sent to the photon calibrator (PCAL). The signal modulates the laser power of the photon calibrator to displace the end test mass (ETM) in a way that mimics a gravitational wave (GW) passing through the detector. The gravitational-wave strain of the detector is analyzed and checked for consistency. A photodiode monitors the reflected light from the test mass to measure the injected signal.

ital control system of the detector at the scheduled time.

Continuous-wave injections are generated in real-time. A streaming time series of simulated gravitational waves from a population of isolated pulsars, described by astrophysical parameters, including the strain amplitude, sky location, and initial frequency, is transmitted to the digital control system of the detector. A driver program coordinates the simultaneous generation and buffering of multiple streams of signals representing spinning neutron stars [24].

The transient and continuous-wave signals in the digital controls system of the detector are sent to an actuator to reconstruct the gravitational-wave strain time series in the detectors' output channel. Two actuation methods were used in aLIGO's first observing.

Hardware injections are carried out by actuating one of the end test masses (ETM) of the interferometer and thus inducing differential interferometer strain variations that simulate the response to an incident gravitational wave. The differential arm length degree of freedom of the interferometer is continuously maintained by a feedback control loop that actuates the longitudinal position of one of the ETM [10]. This feedback control loop suppresses the ETM displacement from noise sources. However, the servo does not suppress the ETM displacement that simulates the injected waveform, since there is a correction for the action of this servo when the strain is injected.

The actuators for this servo are electrostatic drive systems that apply forces via fringing field gradients from electrodes patterned onto a reaction mass separated by a few millimeters from the back surface of the ETM [16, 17]. These actuators were also used at the beginning of aLIGO's first observing run for injecting simulated signals, including the waveforms for the GW150914 and stochastic background hardware injection analyses.

However, the actuation range available for hardware injections is restricted because they are part of the differential arm length servo which consumes a significant fraction of their total actuation range in maintaining stable servo operation. In order to reconstruct a larger parameter space of waveforms, for example binary black hole and/or neutron star mergers at closer distances, we transitioned to a new actuation method for hardware injections.

We currently use a photon calibration system to simulate the displacement of the ETM from a gravitational-wave signal, this is depicted on the right of Fig. 1. A photon calibrator system uses an auxiliary, power-modulated laser with two beams impinging on the ETM located at the end of the  $x$ -arm of the interferometer. The photon calibrator on the other arm, the  $y$ -arm, is used for calibrating the detector output [18]. The two beams are diametrically opposed on the surface of the ETM, balanced in power, and positioned to minimize unintended torques and deformations of the surface which could cause errors in the expected displacement.

The aLIGO photon calibrators employ a feedback control system referred to as the "optical follower servo" [18]. This servo, with a bandwidth of  $\sim 100$  kHz, facilitates simulated signal injection via ETM actuation. This ensures that the laser output power modulation closely follows the analog voltage waveform injected at the servo input.

Digital infinite impulse response (IIR) compensation filters, called the "inverse actuation filters," convert the requested interferometer strain signal (a digital signal) into an estimate of the photon calibrator optical follower servo input signal (an analog signal) required to achieve the desired length actuation. There is an analogous set of filters for the electrostatic drive system, however, we focus on the photon calibrators here. These filters are de-

signed to compensate for a several factors. There is compensation for: (i) the force-to-length transfer function of the suspended ETM, (ii) the signal conditioning electronics that includes a digital anti-imaging filter, the digital to analog converter gain, and an analog anti-imaging filter, and (iii) the optical follower servo transfer function. The digital IIR filters allowed by the aLIGO control system must be causal. Therefore they have known, but uncompensated, delays that we take into account during injection recovery.

The digital signals from the transient and continuous-wave injection pathways are passed through the inverse actuation filters, summed, and sent to the photon calibrator; see Fig. 1. Sporadic, unintended interruptions occurred in the Hanford injection system during aLIGO's first observing run, in which the buffering failed to keep up with real-time injection. The cause was not tracked down because of the unpredictable timing of the interruptions, but the drop-outs may be related to periods of high traffic on the controls system computer network. The sudden termination introduces a step function to the inverse actuation filters that has a large response at high frequencies. In the future, the effect of these dropouts, should they recur, will be mitigated by the use of point-by-point, Fourier-domain inverse actuation functions, using a separate, constant coefficient for each of the injected isolated pulsars, all of which are extremely narrowband. This is shown in the continuous-wave injection pathway in Fig. 1. Transient injections were not affected. Guardian sets the gain after the inverse actuation filters to zero while there is no active transient injection so unintended signals do not propagate into the detector data.

The strain actually injected into the interferometer is determined using the photon calibrator read-back signal generated by a power sensor that monitors the laser light reflected from the ETM; shown at the bottom of Fig. 1. The output of this sensor is converted to injected interferometer strain using the read-back filter that compensates for the force-to-length transfer function as well as digital and analog filters in the signal read-back pathway. However, in the case of hardware injections, the excitation channel is calibrated by taking a transfer function measurement between the excitation channel and the read-back photodetectors. This transfer function is then incorporated within the inverse actuation filters. This provides a calibration accuracy on the order of a few percent, sufficient for the hardware injection analysis. However, for better calibration accuracy, we can compare the recovered signal and the injected signal as measured by the read-back photodetector.

There are some limitations to the photon calibrator system. First, the photon calibrator has a limited actuation strength, Fig. 2 shows the maximal displacement of the ETM using the photon calibrator system. The aLIGO photon calibrator can provide up to  $\sim 1$  W of peak power, but the force-to-length response of the ETM transfer function scales as the inverse-square of frequency [25]. Thus, the photon calibrator is limited in

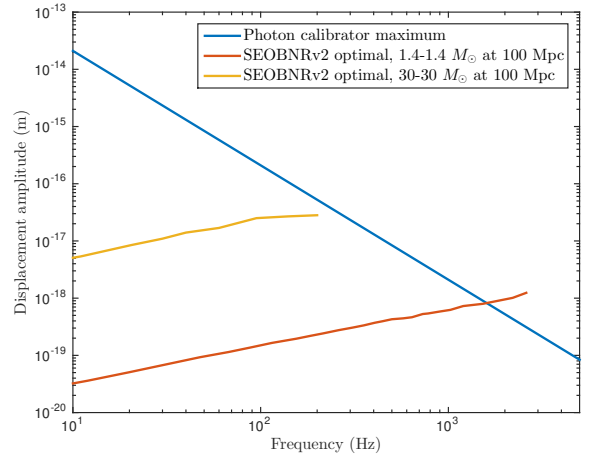


FIG. 2: The maximum displacement of an ETM using the photon calibrator (blue). The maximum displacement of the ETM required for two compact binary waveforms that contain an inspiral, merger, and ringdown are shown for reference; a 30-30  $M_{\odot}$  binary at 100 Mpc (yellow) and 1.4-1.4  $M_{\odot}$  binary at 100 Mpc (red) were generated using the SEOBNRv2 approximant [26]. Note that the required displacement for the 1.4-1.4  $M_{\odot}$  binary exceeds the maximal photon calibrator displacement at high frequencies, however, an inspiral-only waveform for a 1.4-1.4  $M_{\odot}$  binary at 100 Mpc would terminate at 1527 Hz and thus be within the actuation range of the photon calibrator.

the amount of induced ETM displacement, especially at higher frequencies. Second, signal fidelity above  $\sim 1$  kHz is limited due to the shape of the anti-imaging filters and the desire to roll off the compensation filters close to the Nyquist frequency such that the compensation filters are not unstable. Nonetheless, the photon calibrator is able to provide precise, calibrated displacements of the ETMs in response to many astrophysical waveforms.

### III. RESULTS

In this section we describe results from hardware injection analysis in aLIGO's first observing run. Hardware injections were used as: (i) an end-to-end test of searches and parameter estimation analyses, (ii) an additional check of the calibration, and (iii) a method to check for cross-couplings to the detectors' output channel. Binary black hole waveforms with parameters similar to GW150914 and GW151225 were used to test modeled and unmodeled analyses described in Section III A and III B. A simulated stochastic gravitational-wave signal was recovered with the analysis described in Section III C. The population of isolated pulsars analysis in Section III D provided an additional check of the calibration; they were used to verify that the overall sign of the detectors' calibration and measure the time delay between the hardware injection excitation channel and

the detectors' output channel. Section III E describes the study that injects a series of sine-Gaussians across the aLIGO frequency range to check for cross-couplings to the detectors' output.

### A. Compact Binary Coalescence

aLIGO observed the first detections of gravitational waves from binary black hole mergers in its first observing run [6, 7]. After a detection, similar gravitational-wave signals were injected into the interferometer data and recovered by search and parameter estimation analyses as a high-level sanity check. Compact binary coalescence searches use matched filtering to correlate aLIGO data with a bank of gravitational-wave templates. Here we consider hardware injections analyzed by the PyCBC search for gravitational waves described in [27]. Parameter estimation analyses were used to analyze the hardware injections and check for consistency with GW150914 and GW151226. We ran the same algorithm used to characterize the detected events [28, 29]. We show the recovery of hardware injections with parameters taken from posterior distributions of parameter estimation results for GW150914 [29] and GW151226 [7, 20].

For GW150914, we injected ten aligned-spin waveforms coherently into the two detectors; the waveforms were generated with the SEOBNRv2 waveform approximant [26]. PyCBC reports a detection statistic  $\hat{\rho}$  [30] that combines information about the matched-filter signal-to-noise ratio  $\rho$  and the degree to which it is consistent with a compact binary signal  $\chi_r^2$  [12]. Fig. 3 shows the  $\chi_r^2$  statistic [12] versus  $\rho$  for maxima in the signal-to-noise ratio time series for the Hanford (H1) and Livingston (L1) detectors. Hardware injections are indicated with squares. Astrophysical events are indicated with stars. Software injections, in which signals are added to the data without any physical actuation, are denoted by crosses. While hardware injections are an important end-to-end test, software injections are useful because we can carry out a large number without perturbing the detector or significantly reducing the duty cycle of the detectors.

The software injections in Fig. 3 are generated from a population of aligned-spin binaries with source-frame component masses between 2 to 98  $M_\odot$  using the SEOBNRv2 waveform approximant [26]. The population of signals is randomly distributed in sky location, orientation, distance, and time. The injection times are within the 39 day period around GW150914 reported in [31]. We see a separation of the software injections with high significance (false-alarm rate  $< 1/100 \text{ yr}^{-1}$ ) and background distributions. All ten GW150914 hardware injections are recovered with high significance.

Ten hardware injections were injected from the GW151226 posterior distributions on January 11, 2016, these are indicated in Fig. 3 with white squares. The GW151226 hardware injections were generated with the precessing waveform approximant IMRPhenomPv2 [32,

33]. Although the Livingston hardware injections are not visibly distinguishable from the background distribution in Fig. 3, seven hardware injections have a highly significant false-alarm rate ( $< 1/100 \text{ yr}^{-1}$ ) when we combine data from both detectors.

Two hardware injections were recovered with  $1/10 \text{ yr}^{-1} > \text{false-alarm rate} > 1/100 \text{ yr}^{-1}$ , a significance comparable to the gravitational-wave candidate LVT151012 ( $1/2 \text{ yr}^{-1}$ ) reported in aLIGO's first observing run [6].

Another hardware injection had a matched-filter signal-to-noise ratio  $< 5.5$  in Livingston. In order to manage computational considerations, the analysis requires a single-detector signal-to-noise ratio of at least 5.5. Thus, this injection was not "detected." The difference between the intended and actual signal-to-noise ratio for this sub-threshold injection in Livingston is consistent with the variation of the matched-filter output in Gaussian noise [34].

If a detection candidate is a true gravitational wave, we should be able to reproduce the morphology of the posterior distributions using the hardware injections. Conversely any significant differences have the potential to highlight discrepancies between the observation and our waveform models. Here we focus on two parameters: chirp mass and sky location.

The chirp mass  $\mathcal{M}$  is defined as

$$\mathcal{M} = \frac{(m_1 m_2)^{3/5}}{(m_1 + m_2)^{1/5}}. \quad (1)$$

Here,  $m_1$  and  $m_2$  are the binary's component masses. The chirp mass is typically the best estimated parameter of a compact binary coalescence signal, since it dominates the phase evolution during inspiral. In Fig. 5 we show for all the GW151226 hardware injections the posterior distributions of the chirp mass minus the respective injected values, using the precessing waveform approximant IMRPhenomPv2 [32, 33]. Most posteriors have comparable width, hardware injections with low signal-to-noise ratio have broader distributions and in one case shows bimodality. The width of the 90% confidence interval for the detector-frame chirp mass for GW151226 is  $\sim 0.12 M_\odot$  [20], which is comparable to that found with the hardware injections.

Sky maps of GW150914 and GW151226 were shared with electromagnetic observatories [35, 36] and are shown in [20, 37]. In Fig. 4, we show a reconstructed Earth-bound coordinate sky map for GW151226 along with maps for two hardware injections. One of the two hardware injections (at GPS time 1136588345.67) has low signal-to-noise ratio and thus spans a larger sky area, although still along the same triangulation ring. The other injection (at GPS time 136592746.63) is instead representative of the typical map: all other maps look similar to this and are not shown to avoid overcrowding.

A previous study used the parameter estimation method above to validate another parameter estimation

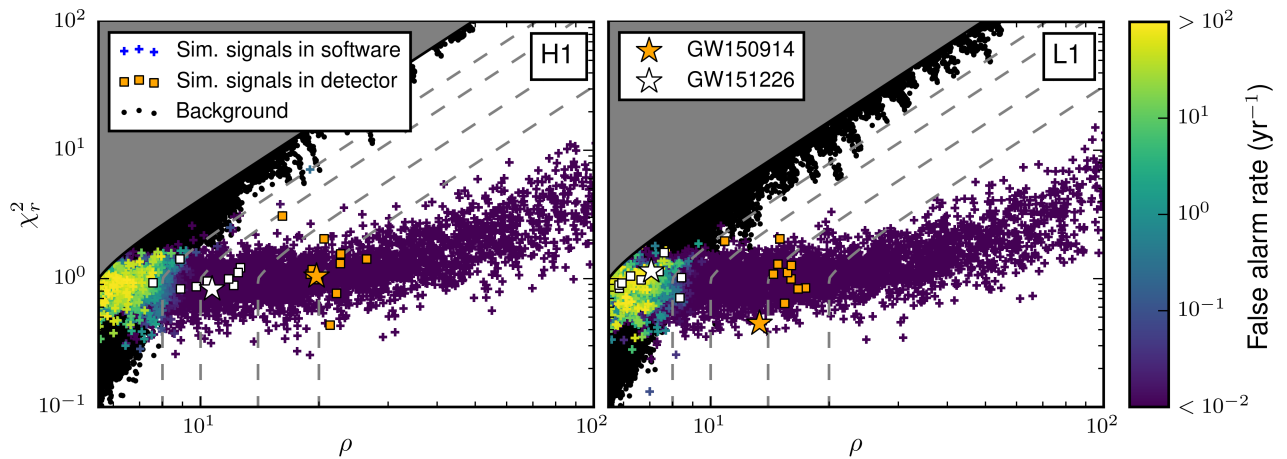


FIG. 3: PyCBC  $\chi_r^2$  statistic versus matched-filter signal-to-noise ratio  $\rho$  for each detector. Software injections are represented as crosses that are colored by false-alarm rate. The gravitational-wave events GW150914 and GW151226 are shown as stars. Hardware injections for GW150914 and GW151226 are represented as boxes. Background distributions (black dots) are plotted; there was a threshold applied indicated by the gray region. Lines of constant detection statistic  $\hat{\rho}$  are shown (gray dashed lines); plotted are  $\hat{\rho} = \{8, 10, 14, 20\}$ .

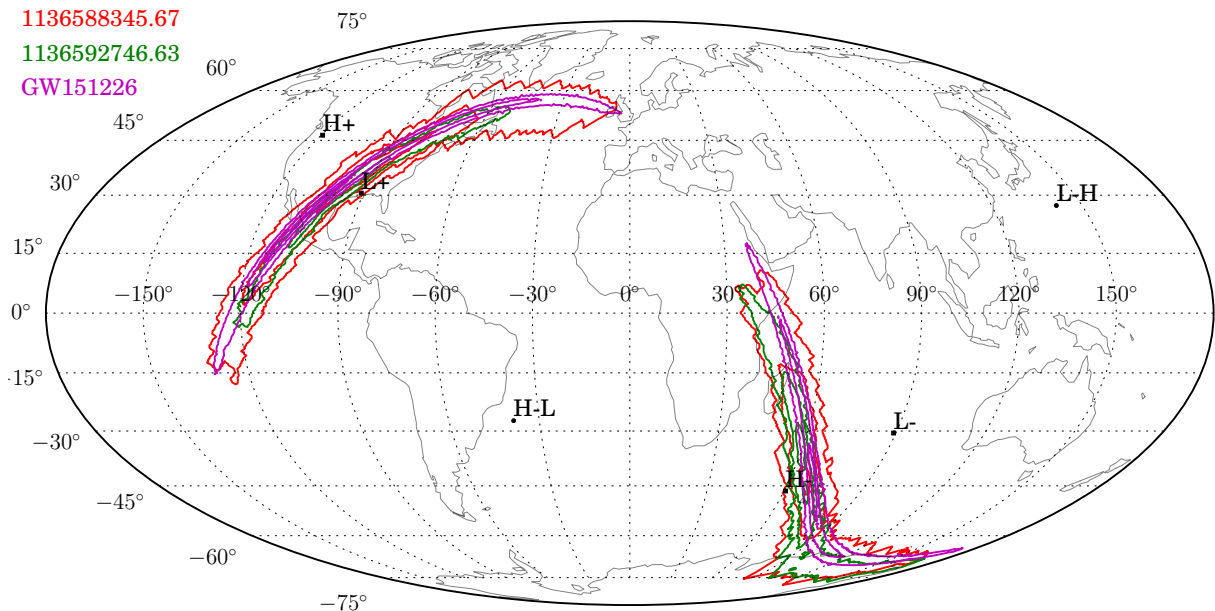


FIG. 4: The 90% confidence interval skymaps for two hardware injection (red and green) and GW151226 (magenta). The skymaps are shown in Earth-bound coordinates. The two hardware injections are chosen to be representative of an average event (green) and a sub-threshold event (red). We notice how all sky maps have support on the same ring of equal time delay between the two aLIGO detectors.

strategy used to interpret GW150914, by directly comparing data to simulations of Einstein's equations [38]. In that study the parameter estimates for GW150914 derived from IMRPhenomPv2 and numerical relativity agreed [38]. This study was repeated comparing hardware injections to numerical relativity, and found poste-

rior distributions in mass and spin were consistent with the IMRPhenomPv2 analysis.



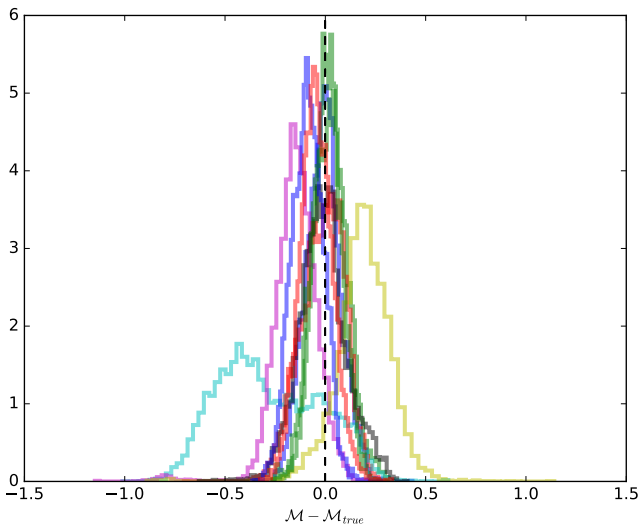


FIG. 5: Posterior distributions for the chirp mass of the GW151226 hardware injections. The true value has been removed to center all distributions around zero. Hardware injections with very low signal-to-noise ratio show large width and in one case bimodality. The bimodal distribution comes from the injection at GPS time 1136588345.67 which is also shown in Fig. 4.

### B. Burst

There are astrophysical sources of gravitational waves that have poorly modeled or unknown waveforms, such as core-collapse supernovae [39]. In order to search for a wide range of unmodeled astrophysical sources, analyses look for short-duration, transient gravitational-wave events referred to as “bursts” [40]. Here, we look at injection recoveries using: Coherent WaveBurst [41], BayesWave [42], and LALInferenceBurst [43, 44]. These analyses produce reconstructed waveforms with minimal assumptions about the waveform morphology. We compare these reconstructions to the injected waveforms of hardware injections.

In addition to the ten GW150914 hardware injections described in Section III A, there were 24 waveforms with physical parameters similar to GW150914 injected. Eight were non-spinning waveforms with equal component masses and a total mass of  $76 M_{\odot}$ ; sixteen were aligned-spin with total masses from  $[70, 80] M_{\odot}$  and mass ratios from 1 to 5. Mass ratio is defined as  $m_1/m_2$  where  $m_1 > m_2$ . The waveforms were generated with the SEOBNRv2 approximant [26].

Since burst searches do not use gravitational-wave templates, they are less sensitive to signals [45]. The burst searches did not recover GW151226, and only recovered a single hardware injection performed to validate that detection. The GW151226 hardware injections are not included in these results.

Coherent WaveBurst identifies coherent events in spectrographic data from the aLIGO detectors constructed

using a wavelet representation. It then reconstructs the gravitational waveform using a likelihood analysis [41]. For signals consistent with compact binary coalescences, it also estimates the system’s chirp mass based on the time-frequency evolution of the signal [46]. The low-latency Coherent WaveBurst search recovered 28 of the 34 total injections. In Fig. 6 we show the recovered versus injected excess power signal-to-noise ratio and chirp mass. Note that the excess power signal-to-noise ratio [41] is distinct from the matched-filter signal-to-noise ratio  $\rho$ .

BayesWave uses a sum of sine-Gaussian wavelets to model the gravitational-wave signal [42]. The reconstruction assumes an elliptically polarized gravitational wave, but no other constraints are imposed [42]. BayesWave investigated the 28 GW150914 hardware injections recovered by Coherent WaveBurst. Previous studies with software injections show that the recovered waveforms produced by BayesWave accurately match injected signals [40]. To measure the overlap between injected and recovered waveforms, we use the network match

$$\text{Match} = \frac{(h_{\text{inj}}|h_{\text{rec}})}{\sqrt{(h_{\text{inj}}|h_{\text{inj}}) \times (h_{\text{rec}}|h_{\text{rec}})}} \quad (2)$$

where  $h_{\text{inj}}$  is the injected waveform,  $h_{\text{rec}}$  is the recovered waveform, and  $(a|b)$  is the noise-weighted inner product summed over all interferometers [42]. The average network match between the injected and reconstructed waveforms is 94%. The 94% match is consistent with the average match found using software injections [40]. An example of a reconstructed waveform is shown in Fig. 7.

Coherent WaveBurst, BayesWave, and LALInferenceBurst provide sky localization estimates as the signal is reconstructed. Fig. 8 demonstrates sky maps for one of the GW150914 hardware injections and GW150914 itself [29]. We see similar support in Earth-bound coordinates, and nearly identical structures around the triangulation rings. The right-hand panels of Fig. 8 highlight this with the posterior distributions for the time delay between the two detectors.

### C. Stochastic

A stochastic gravitational-wave background is expected to arise from the superposition of many events, each of which are too weak to resolve, but which combine to create a low-level signal [21]. By cross correlating data from two or more detectors, it is possible to detect low-level correlations hidden beneath the detectors’ noise [47]. The stochastic background from unresolved binary black holes is a particularly promising source, potentially within reach of advanced detectors [48]. On October 23, 2015, a stochastic gravitational-wave background signal was simultaneously injected into both detectors. The 600 s-long signal corresponded to an isotropic Gaussian background.

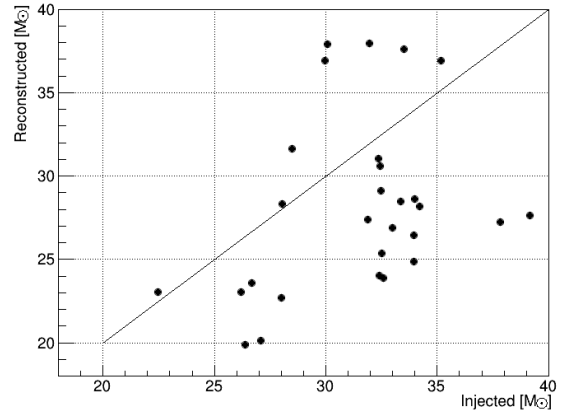
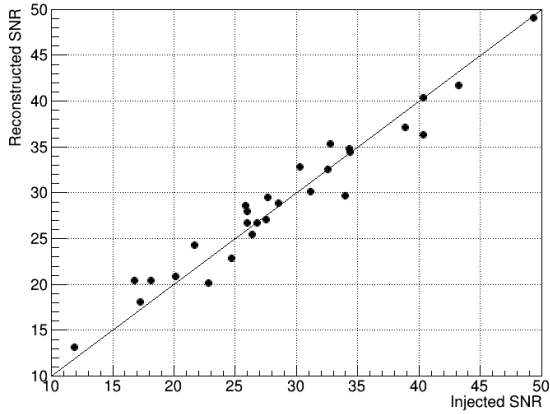


FIG. 6: The 28 recovered hardware injections by the low-latency Coherent WaveBurst search. *Left*: Recovered excess power signal-to-noise ratio (Reconstructed SNR) versus injected excess power signal-to-noise ratio (Injected SNR). *Right*: Recovered chirp mass (Reconstructed) versus injected chirp mass (Injected).

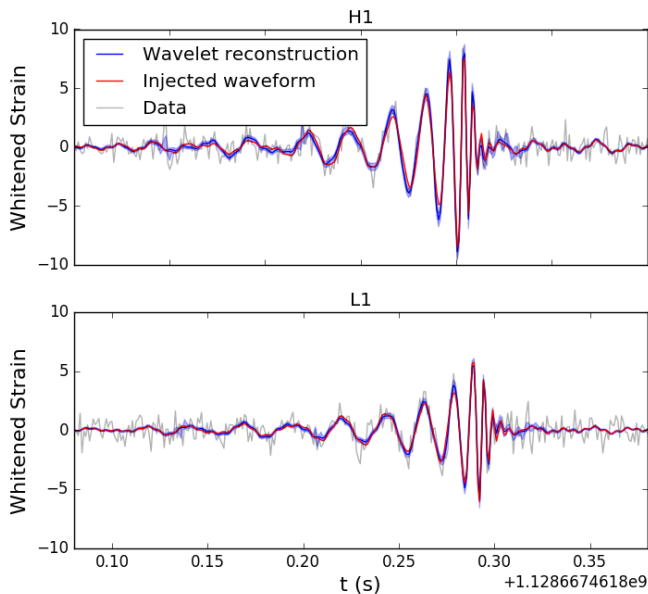


FIG. 7: BayesWave median reconstruction and 90% credible interval (blue) and the injected waveform (red), time is shown on the  $x$ -axis and whitened strain on the  $y$ -axis. The data has been whitened using the estimated noise curve from the time of the injection. The network match for this waveform is 98%.

The strength of a stochastic gravitational-wave signal is parameterized by the fractional contribution of the energy density in gravitational waves to close the Universe [47]:

$$\Omega_{\text{GW}}(f) = \frac{1}{\rho_c} \frac{d\rho_{\text{GW}}}{d \ln f}. \quad (3)$$

Here,  $\rho_c$  is the critical energy density of the Universe,  $f$  is frequency, and  $d\rho_{\text{GW}}$  is the energy density between  $f$  and  $f + df$ . The injected signals were chosen such that

$\Omega_{\text{GW}}(f) = 8.7 \times 10^{-5}$ . This corresponds to a strain power spectral density of

$$S_h(f) = \frac{3H_0^2}{10\pi^2} \frac{\Omega_{\text{GW}}(f)}{f^3} = \left(2.9 \times 10^{-23} \text{ Hz}^{-1/2}\right)^2 \left(\frac{25 \text{ Hz}}{f}\right)^3 \quad (4)$$

where  $H_0$  is the Hubble constant.

We carried out a cross-correlation search following the standard procedure [49]. The data was split into 50%-overlapping, 60 s intervals, and utilizing coarse-grained 0.25 Hz-wide frequency bins, we recovered an  $\Omega_{\text{GW}}(f)$  of  $(8.8 \pm 0.6) \times 10^{-5}$ , consistent with the injected value. The recovered signal is shown in Fig. 9. The  $y$ -axis shows the recovered signal as a function of the time lag between the detectors. A peak at zero, and the absence of structure at other times, shows that the signal is recovered as expected.

#### D. Continuous Wave

The recovery of hardware injections is used by continuous-wave searches as an end-to-end validation of the analyses in the presence of instrumental artifacts and imperfect instrument calibration. Coherent searches for known pulsars are sensitive to deviations from the injected signal since a small bandwidth around the gravitational-wave frequency is integrated for months or years [22]. These searches have the capability of monitoring the self-consistency of the interferometer calibration and, in particular, the long-term stability of absolute phase recovery. Continuous-wave searches can be implemented using radiometer [50, 51] or Bayesian methods [22]. Here, we consider a coherent search based on Bayesian recovery of signal parameters [22] to validate



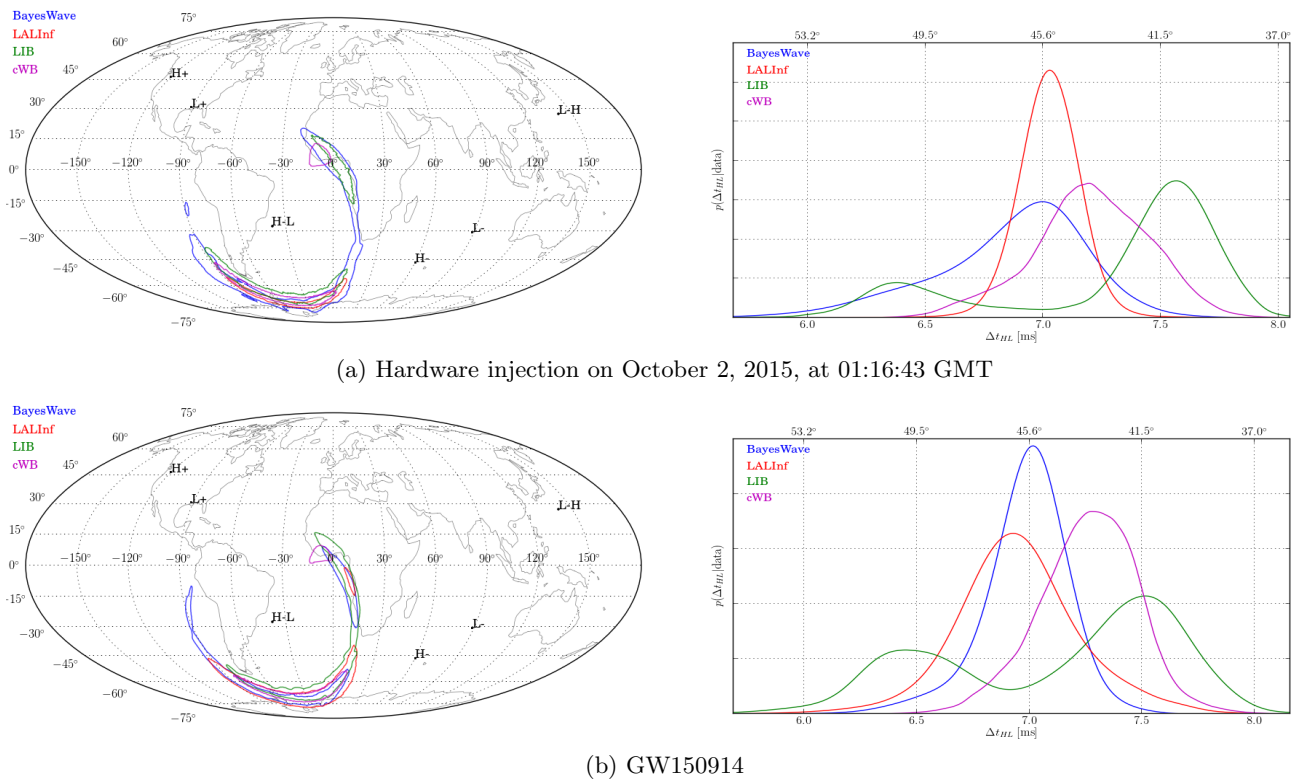


FIG. 8: Sky localizations estimates from burst analyses: BayesWave, Coherent WaveBurst (cWB), and LALInferenceBurst (LIB). We include the parameter estimation analysis from Section III A (LALInf) for comparison [29]. *Left*: We show the localization maps in Earth-bound coordinates for a GW150914 hardware injection and GW150914 itself. *Right*: To highlight the similar positions relative to the detectors the marginal distributions for the time delay between the two detectors is shown.

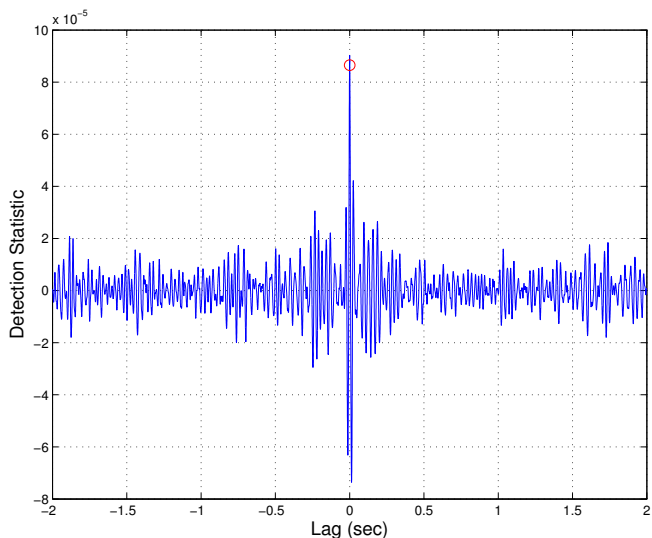


FIG. 9: Recovered stochastic signal as a function of lag time between detectors (blue). The injected signal is represented with a red circle. The peak of the recovered signal intersects with the injection at zero lag, indicating a successful recovery.

the fidelity of hardware injections. This analysis can be used to cross-check many elements of the instrument calibration, including proper coherence of data from interferometers separated by thousands of kilometers, which are sensitive to timing errors. Hardware injection recovery provides a sanity check of the overall sign of the detectors’ calibration.

During aLIGO’s first observing run, there were 15 isolated pulsars streaming in real-time with frequencies ranging from 12 – 1991 Hz. Fig. 10 shows the posterior for strain amplitude  $h_0$  for a pulsar, which has a signal frequency near 108.9 Hz and a nearly linear polarization. The signal is recovered with an amplitude consistent with the intended strength, within calibration and actuation uncertainties. Similarly, Fig. 10 also shows the recovered phase constant for this injection; again, consistency with expectation is observed, given an uncompensated time delay. The time delay is from the actuation pathway between the hardware injection excitation channel and the detector output channel. This time delay can be measured with the population of isolated pulsars.

Fig. 11 and 12 show a summary of the agreement between recovered and intended amplitude and phase for the 14 injections with sufficient signal-to-noise ratio to permit recovery. Instrumental noise at the lowest-frequency injection (12 Hz) proved too large to permit signal recovery. There is evidence of a constant uncompensated time delay of about  $150 \mu\text{s}$  in the time-domain actuation, which manifests as a phase delay increasing linearly with injection frequency in Fig. 12. In the future, a compensating timing advance will be included in the inverse actuation filter, and the pulsars’ amplitudes will be increased for more precise and rapid validation of the hardware injection signal.

## E. Detector Characterization

Noise artifacts in aLIGO data adversely affect the output of gravitational-wave search analyses [8, 52]. In searches for transient gravitational waves, some periods of time are excluded from the analysis to remove periods of poor data quality and known transient noise. These are known as “data quality vetoes” [8, 52]. Removing periods of time with excess noise improves the performance of gravitational-wave searches [8, 52]. Some of these data quality vetoes are derived from information recorded in auxiliary channels. Auxiliary channels include instrumental channels that record degrees of freedom of the interferometer and its isolation systems as well as channels that monitor the environmental conditions around the instrument [53]. The environmental monitoring system includes seismic, acoustic, and electromagnetic data.

To avoid discarding true gravitational-wave signals, any auxiliary channels used for vetoes are first checked to ensure that they do not respond to gravitational-wave-like signals; i.e., changes in differential arm-length. This process is referred to as a “safety check,” since a channel that has no sensitivity to gravitational waves is considered “safe” for use when constructing a veto. To test whether auxiliary channels respond to differential arm-length changes, three sets of 12 loud (matched-filter signal-to-noise ratios  $> 100$ ) transient hardware injections were performed at both detectors, and the auxiliary channel data were examined both qualitatively and quantitatively for signs of coupling.

Spectrograms were manually inspected at the time of hardware injections. These signals were very strong and clear, with high signal-to-noise ratio, in channels that were expected to record differential displacement, e.g. interferometer differential sensing and actuation, and closely related degrees of freedom. No signs of coupling were found in thousands of other auxiliary channels, indicating that they may be used to construct vetoes. Thousands of time-frequency representations of auxiliary channels were also inspected at the times of GW150914 and GW151226 with the same outcome [8].

Loud hardware injections were used to statistically assess the coupling. An algorithm based on a transformation using sine-Gaussians [54] was used to identify and parameterize noise transients by their time, frequency, signal-to-noise ratio, etc. The time of noise transient is compared with the times of the loud hardware injections. For each channel, the number of noise transients that occurred within 100 ms of loud injections are counted and compared to the number that would be expected based on chance [55]. For any channel exhibiting a higher number of overlaps than expected by chance, the time-frequency behavior of the raw data is further investigated to see if there is a plausible connection. We find that only obviously related channels, such as those in the sensing and actuation chain for the differential length control loop, were sensitive to the loud hardware injections.

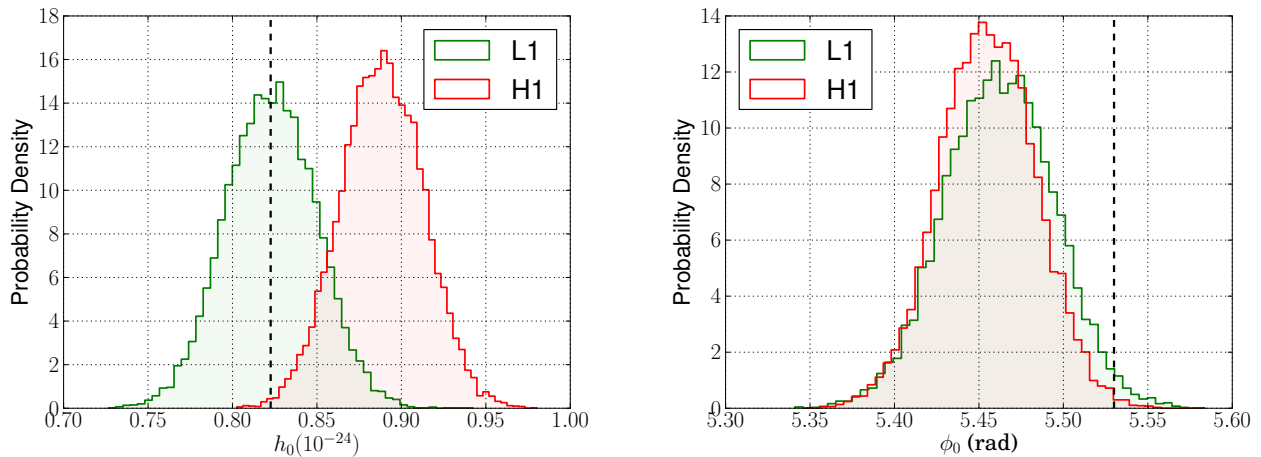


FIG. 10: Posterior probability density functions for the recovered strain amplitude and phase constant for the pulsar at 108.86 Hz. The dashed vertical line indicates the intended injection amplitude and phase in radians. The red and green curves indicate the separately recovered amplitudes and phases for the Hanford and Livingston interferometers, respectively. The apparent residual discrepancies in amplitude and phase fall within the uncertainties of the actuation system used for the injections.

#### IV. CONCLUSIONS

This paper presents the aLIGO hardware injection system infrastructure for injecting signals into the interferometers and results from aLIGO's first observing run. Hardware injections were used for validating analyses after a gravitational-wave detection, an additional check of the calibration, and detector characterization.

For GW150914 and GW151226, sets of binary black hole merger waveforms with similar parameters were injected to validate the search and parameter estimation analyses. The injected waveforms were checked for consistency with the recovered signals, including signal-to-noise ratio, chirp mass, and sky position. Similarly, the stochastic background and continuous-wave searches used simulated waveforms as an end-to-end test.

Astrophysical signals would differ by a sign and not be recovered correctly, if the sign of the calibration between the two sites differed. The continuous-wave injections

were used to validate that the sign of the calibration between the aLIGO detectors was correct. We were also able to measure the time delay of the hardware injection pathway and check that it was consistent with the predicted value from the calibration model.

After each gravitational-wave detection, we carried out a study to check for cross-couplings with the detectors' output channel. For both GW150914 and GW151226 we only found traces of the injected signals in channels we expected to cross-couple with differential displacement. These channels were excluded from data quality veto studies that were used to improve the performance of analyses.

In the future, we plan to exclusively use the photon calibrators to inject simulated gravitational waves. Future work on the hardware injection system includes using point-by-point, Fourier-domain inverse actuation functions for each of the injected isolated pulsars to mitigate the effect of data dropouts.

- 
- [1] J. Aasi et al., *Class. Quant. Grav.* **32**, 074001 (2015).
  - [2] Acernese, F. and others, *Class. Quant. Grav.* **32**, 024001 (2015).
  - [3] H. Grote and the LIGO Scientific Collaboration, *Class. Quant. Grav.* **27**, 084003 (2010).
  - [4] Y. Aso, Y. Michimura, K. Somiya, M. Ando, O. Miyakawa, T. Sekiguchi, D. Tatsumi, , and H. Yamamoto, *Phys. Rev. D* **88**, 043007 (2013).
  - [5] B. Iyer et al., *LIGO-India Tech. Rep.* (2011), URL <https://dcc.ligo.org/LIGO-M1100296/public>.
  - [6] B. P. Abbott et al., *Phys. Rev. Lett.* **116**, 061102 (2016).
  - [7] B. P. Abbott et al., *Phys. Rev. Lett.* **116**, 241103 (2016).
  - [8] B. P. Abbott, R. Abbott, T. D. Abbott, M. R. Abernathy, F. Acernese, K. Ackley, M. Adamo, C. Adams, T. Adams, P. Addesso, et al., *Classical and Quantum Gravity* **33**, 134001 (2016), 1602.03844.
  - [9] J. Aasi et al., *Class. Quant. Grav.* **32**, 115012 (2015).
  - [10] B. P. Abbott et al. (LIGO Scientific) (2016), 1602.03845.
  - [11] E. Thrane, N. Christensen, R. M. S. Schofield, and A. Effler, *Phys. Rev. D* **90**, 023013 (2014).
  - [12] B. Allen (2005).
  - [13] J. Abadie et al., *Phys. Rev. D* **85**, 082002 (2012).
  - [14] J. Abadie et al. (VIRGO, LIGO), *Phys. Rev. D* **81**, 102001 (2010), 1002.1036.
  - [15] B. P. Abbott et al. (Virgo, LIGO Scientific), *Phys. Rev. Lett.* **116**, 131103 (2016), 1602.03838.

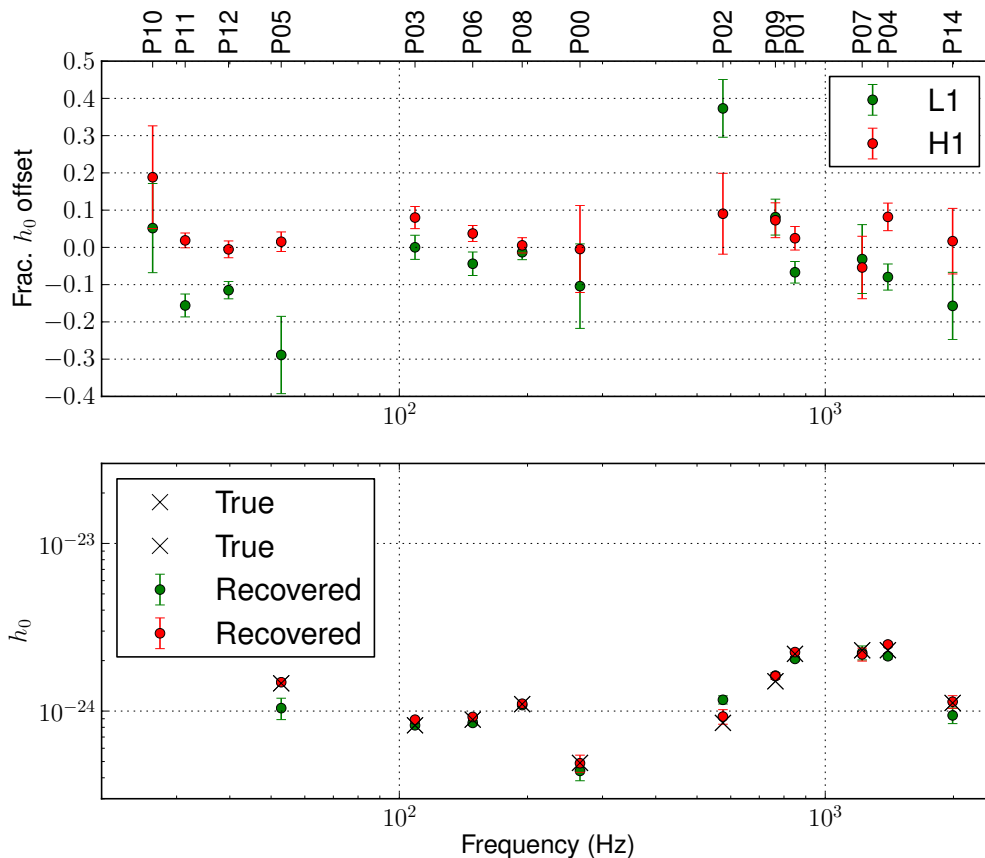


FIG. 11: Comparisons of recovered signal amplitudes for the Hanford and Livingston signals for the 15 recovered continuous-wave injections (P00-P14). *1st panel*: Fractional amplitude difference [(recovered minus injected)/injected]. *2nd panel*: Amplitude values (recovered and injected).

- [16] N. Lockerbie, *Electrostatic driver e3074 user manual* (2011), URL <https://dcc.ligo.org/T1100231>.
- [17] L. Carbone et al., *Class. Quant. Grav.* **29**, 115005 (2016).
- [18] S. Karki et al., ArXiv e-prints (2016), 1608.05055.
- [19] B. P. Abbott et al. (Virgo, LIGO Scientific) (2016), 1607.07456.
- [20] B. Abbott et al., *Binary Black Hole Mergers in the first Advanced LIGO Observing Run* (2016), URL <https://dcc.ligo.org/LIGO-P1600088>.
- [21] M. Maggiore, *Physics Reports* **331**, 283 (2000).
- [22] J. Aasi et al. (LIGO Scientific), *Astrophys. J.* **785**, 119 (2014), 1309.4027.
- [23] J. Rollins, *Advanced LIGO Guardian Documentation* (2015), URL <https://dcc.ligo.org/LIGO-T1500292>.
- [24] LSC Data Analysis Software Working Group, *LALSuite*, <https://www.lsc-group.phys.uwm.edu/daswg/projects/lalsuite.html>, URL <https://www.lsc-group.phys.uwm.edu/daswg/projects/lalsuite.html>.
- [25] E. Goetz, P. Kalmus, S. Erickson, R. L. Savage, G. Gonzalez, K. Kawabe, M. Landry, S. Marka, B. O'Reilly, K. Riles, et al., *Classical and Quantum Gravity* **26**, 245011 (2009), URL <http://stacks.iop.org/0264-9381/26/i=24/a=245011>.
- [26] A. Taracchini et al. (2012).
- [27] S. Usman et al., *An improved pipeline to search for gravitational waves from compact binary coalescence* (2015).
- [28] J. Veitch et al. (2015).
- [29] B. P. Abbott et al., *Phys. Rev. Lett.* **116**, 241102 (2016).
- [30] S. Babak et al. (2013).
- [31] B. P. Abbott et al., *Phys. Rev. D* **93**, 122003 (2016).
- [32] P. Schmidt et al. (2015).
- [33] M. Hannam et al. (2014).
- [34] D. Brown, Ph.D. thesis, U. Wisconsin-Milwaukee (2004), URL <https://inspirehep.net/record/673638/files/arXiv:0705.1514.pdf>.
- [35] L. Singer et al. (2015), URL <http://gcn.gsfc.nasa.gov/other/GW150914.gcn3>.
- [36] L. Singer et al. (2015), URL <http://gcn.gsfc.nasa.gov/other/GW151226.gcn3>.
- [37] L. S. Collaboration and the Virgo Collaboration (2016).
- [38] B. P. Abbott et al. (Virgo, LIGO Scientific), *Phys. Rev. D* **94**, 064035 (2016), 1606.01262.
- [39] F. C. L. and B. K. C., *Gravitational waves from gravitational collapse* (2011).
- [40] B. P. Abbott et al., *Phys. Rev. D* **93**, 122004 (2016).
- [41] S. Klimenko, G. Vedovato, M. Drago, F. Salemi, V. Tiwari, G. A. Prodi, C. Lazzaro, K. Ackley,

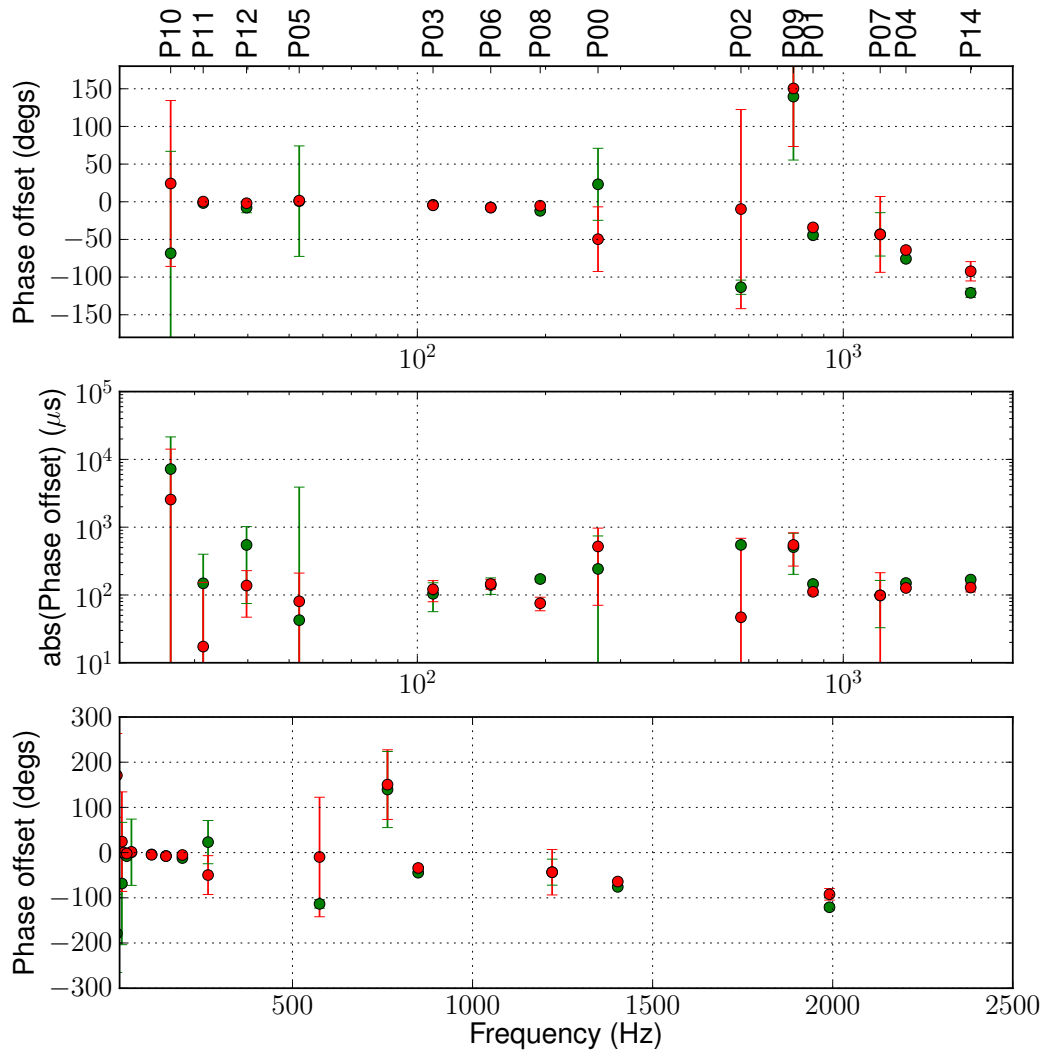


FIG. 12: Comparisons of recovered signal phases for the Hanford and Livingston signals for the 15 recovered continuous-wave injections (P00-P14). *1st panel*: Phase difference (degrees) [recovered minus true]. *2nd panel*: Conversion of phase difference magnitude to time difference. *3rd panel*: Same as 3rd panel but with linear horizontal scale, to indicate the roughly linear dependence of residual phase difference, consistent with a constant uncompensated time delay.

- S. Tiwari, C. F. Da Silva, et al., Phys. Rev. D **93**, 042004 (2016), URL <http://link.aps.org/doi/10.1103/PhysRevD.93.042004>.
- [42] N. J. Cornish and T. B. Littenberg, Class. Quant. Grav. **32**, 135012 (2015), 1410.3835.
- [43] J. Veitch et al., Phys. Rev. **D91**, 042003 (2015), 1409.7215.
- [44] S. J., Bayesian Anal. **2006** (????).
- [45] B. A. et al., in prep. (????).
- [46] V. Tiwari, S. Klimenko, V. Nacula, and G. Mitselmakher, Classical and Quantum Gravity **33**, 01LT01 (2016).
- [47] B. Allen and J. D. Romano, Phys. Rev. D **59**, 102001 (1999).
- [48] B. P. Abbott et al., Phys. Rev. Lett. **116**, 131102 (2016).
- [49] J. Aasi et al. (The LIGO Scientific and Virgo Collaborations), Phys. Rev. Lett. **113**, 231101 (2014).
- [50] S. W. Ballmer, Class. Quant. Grav. **23**, S179 (2006), gr-qc/0510096.
- [51] B. P. Abbott et al. (VIRGO, LIGO), Phys. Rev. Lett. **107**, 271102 (2011).
- [52] J. Aasi, J. Abadie, B. P. Abbott, R. Abbott, T. Abbott, M. R. Abernathy, T. Accadia, F. Acernese, C. Adams, T. Adams, et al., Classical and Quantum Gravity **32**, 115012 (2015), 1410.7764.
- [53] A. Effler et al., **32**, 035017 (2015).
- [54] S. Chatterji, L. Blackburn, G. Martin, and E. Katsavounidis, Classical and Quantum Gravity **21**, S1809 (2004).
- [55] J. R. Smith et al., Class. Quantum Grav. **28**, 235005 (2011).